



**TEST REPORT**  
**IEC 61010-1**  
**Safety requirements for electrical equipment for measurement,**  
**control, and laboratory use**  
**Part 1: General requirements**

**Report Number** .....: SHES190101009901  
**Date of issue** .....: 2019-04-19  
**Total number of pages**.....: 86

**Name of Testing Laboratory preparing the Report**.....: SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

**Applicant's name** .....: Hangzhou Hikvision Digital Technology Co., Ltd  
**Address**.....: No.555 Qianmo Road, Binjiang District, Hangzhou 310052, China

**Test specification:**  
**Standard**.....: IEC 61010-1:2010, AMD1:2016  
**Test procedure** .....: SGS-CSTC  
**Non-standard test method** .....: N/A

**Test Report Form No.** .....: IEC61010\_1L  
**Test Report Form(s) Originator** ....: VDE Testing and Certification Institute  
**Master TRF**.....: 2017-10-20

**Copyright © 2017 IEC System of Conformity Assessment Schemes for Electrotechnical Equipment and Components (IECEE System). All rights reserved.**

This publication may be reproduced in whole or in part for non-commercial purposes as long as the IECEE is acknowledged as copyright owner and source of the material. IECEE takes no responsibility for and will not assume liability for damages resulting from the reader's interpretation of the reproduced material due to its placement and context.

If this Test Report Form is used by non-IECEE members, the IECEE/IEC logo and the reference to the CB Scheme procedure shall be removed.

**This report is not valid as a CB Test Report unless signed by an approved CB Testing Laboratory and appended to a CB Test Certificate issued by an NCB in accordance with IECEE 02.**

**General disclaimer:**

The test results presented in this report relate only to the object tested.  
This report shall not be reproduced, except in full, without the written approval of the Issuing CB Testing Laboratory. The authenticity of this Test Report and its contents can be verified by contacting the NCB, responsible for this Test Report.

<b>Test item description</b> ..... :	Handheld Thermography Camera	
<b>Trade Mark</b> ..... :	HIKVISION	
<b>Manufacturer</b> .....	Same as applicant	
<b>Model/Type reference</b> ..... :	See page 7-8	
<b>Ratings</b> ..... :	5 Vd.c., 1,1 A, 5,5 W, Class III	
<b>Responsible Testing Laboratory (as applicable), testing procedure and testing location(s):</b>		
<input checked="" type="checkbox"/>	<b>Testing Laboratory:</b>	SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.
	<b>Testing location/ address</b> .....	588 West Jindu Road, Xinqiao Songjiang 201612 Shanghai, China.
	<b>Tested by (name, function, signature)</b> ..... :	Michael Xu
	<b>Approved by (name, function, signature)</b> .. :	Lancer Lei
<input type="checkbox"/>	<b>Testing procedure: CTF Stage 1:</b>	
	<b>Testing location/ address</b> .....	
	<b>Tested by (name, function, signature)</b> ..... :	
	<b>Approved by (name, function, signature)</b> .. :	
<input type="checkbox"/>	<b>Testing procedure: CTF Stage 2:</b>	
	<b>Testing location/ address</b> .....	
	<b>Tested by (name + signature)</b> ..... :	
	<b>Witnessed by (name, function, signature)</b> . :	
	<b>Approved by (name, function, signature)</b> .. :	
<input type="checkbox"/>	<b>Testing procedure: CTF Stage 3:</b>	
<input type="checkbox"/>	<b>Testing procedure: CTF Stage 4:</b>	
	<b>Testing location/ address</b> .....	
	<b>Tested by (name, function, signature)</b> ..... :	
	<b>Witnessed by (name, function, signature)</b> . :	
	<b>Approved by (name, function, signature)</b> .. :	
	<b>Supervised by (name, function, signature)</b> :	



List of Attachments (including a total number of pages in each attachment)		
Document No.	Documents included / attached to this report (description)	Page No.
Attachment 1	Photos documents	8

Documents referenced by this report (available on request):		
Document Name or No.	Documents description	Page No.
-		

**Summary of testing:**

The sample(s) tested complies with the requirements of IEC 61010-1:2010, EN 61010-1:2010.  
 The laser part for the test sample was tested and complied with laser class 2 as per IEC 60825-1:2014 and EN 60825-1:2014.

When determining the test conclusion, the Measurement Uncertainty of test has been considered.

Unless otherwise, all tests were performed on model DS-2TP31-03AUF was considered as worst condition.  
 The building-in lithium battery pack was tested and complied with IEC 62133:2012 and EN 62133:2012

Heating test (4.5):  
 T<sub>ma</sub> = 50°C (declared by manufacturer)

K-type thermocouple used for temperature measurement.

Clause	Comment
4.4 Testing in single fault conditions 5.1.3 Mains supply 5.3 Durability of markings 6.2 Determination of ACCESSIBLE parts 7.2 Sharp edges 8.2.1 Static test 8.3 Drop test 10.4 Conduct of temperature tests 11.2 Cleaning 13.2.2 Batteries and battery charging 14 COMPONENTS AND SUBASSEMBLIES	SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. 588 West Jindu Road, Xinqiao, Songjiang, 201612 Shanghai, China

<b>Test Report History:</b> This report may consist of more than one report and is only valid with additional or previous issued reports:	
Report Ref. No.	Item
Original report	
<b>Tests performed (name of test and test clause):</b> -	<b>Testing location:</b> -
<b>Summary of compliance with National Differences (List of countries addressed):</b> EU Group Differences (EN 61010-1:2010+A1:2016)  The text of the International Standard IEC 61010-1:2010 was approved by CENELEC as a European Standard without any modification.  The product fulfils the above requirements.  <input checked="" type="checkbox"/> <b>The product fulfils the requirements of EN 61010-1:2010+A1:2016</b>	

<p><b>Copy of marking plate:</b></p> <p>The artwork below may be only a draft. The use of certification marks on a product must be authorized by the respective National Certification Body that own these marks.</p> <div style="text-align: center;"> <p> <b>HIKVISION</b>                      Handheld Thermography Camera                      Model: DS-2TP31-03AUF                      I/P: 5V 1.1A, 5.5W                      SN: 1234567AB ABCDEFG                      SV: V5.5.16Build181224 EN 60825-1: 2014                 </p> <div style="border: 1px solid black; padding: 2px; width: fit-content; margin: 0 auto;">                     Made in China                      Manufacturer: Hangzhou Hikvision Digital Technology Co., Ltd.                      Address: No. 555 Qianmo Road, Binjiang District, Hangzhou 310052, China                      This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.                 </div> <div style="border: 1px solid black; padding: 2px; width: fit-content; margin: 0 auto;">                     LASER RADIATION                      DO NOT STARE INTO BEAM                      CLASS 2 LASER PRODUCT                      λ=650nm, &lt;1mW                      EN 60825-1 : 2014                 </div> </div> <p>Remark:</p> <ol style="list-style-type: none"> <li>1) The Height of CE logo shall not be less than 5 mm; Height of WEEE logo shall not be less than 7 mm;</li> <li>2) As declared by the applicant, the importer (and manufacturer, if it is different)'s name, registered trade name or registered trade mark and the postal address will be marked on the products before being place on the market. The contact details shall be in a language easily understood by end-users and market surveillance authorities.</li> <li>3) The marking plates for other models are of the same pattern except model no.</li> </ol>
---

<b>Test item particulars:</b>	
Type of item .....	Measurement
Description of equipment function.....	Handheld thermography camera
Connection to MAINS supply .....	Battery operated
Overvoltage category .....	N/A
POLLUTION DEGREE.....	2
Means of protection .....	Class III
Environmental conditions .....	Extended (Specify): -10 °C to 50 °C Less than 90% Rh
For use in wet locations.....	No
Equipment mobility.....	Hand-held
Operating conditions.....	Continuous
Overall size of equipment (W x D x H).....	196mm x 59mm x 78mm
Mass of equipment (kg).....	0,30
Marked degree of protection to IEC 60529 .....	N/A
<b>Possible test case verdicts:</b>	
- Test case does not apply to the test object .....	N/A (Not Applicable)
- Test object does meet the requirement.....	P (Pass)
- Test object does not meet the requirement .....	F (Fail)
<b>Testing:</b>	
Date of receipt of test item.....	2019-01-10
Date (s) of performance of tests .....	2019-01-15 to 2019-02-10
<b>General remarks:</b>	
<p>The test results presented in this report relate only to the object tested.            This report shall not be reproduced, except in full, without the written approval of the issuing testing laboratory.            "(see ENCLOSURE #)" refers to additional information appended to the report.            "(see Form A.xx)" refers to a Table appended to the report.            Bottom lines for measurement Tables Forms A.xx are optional if used as record.</p> <p><b>Throughout this report a <input checked="" type="checkbox"/> comma / <input type="checkbox"/> point is used as the decimal separator.</b></p> <p>This document is issued by the company under its General Conditions of Service accessible at <a href="http://www.sgs.com/terms_and_conditions.htm">http://www.sgs.com/terms_and_conditions.htm</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined there in. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.</p> <p>Unless otherwise stated: (a) the results shown in this document refer only to the sample(s) tested and (b) such sample(s) are retained for 1 month. This document cannot be reproduced except in full, without prior approval of the company.</p>	

**Manufacturer's Declaration per sub-clause 4.2.5 of IEC 60335-1:**

The application for obtaining a CB Test Certificate includes more than one factory location and a declaration from the manufacturer stating that the sample(s) submitted for evaluation is (are) representative of the products from each factory has been provided..... :

- Yes
- Not applicable

**When differences exist; they shall be identified in the general product information section.**

**Name and address of factory (ies) .....**: Hangzhou Hikvision Technology Co., Ltd.  
 No. 700, Dongliu Road, Binjiang District, Hangzhou City, Zhejiang, 310052, China.

**General product information and other remarks:**

Description of unit:

Functions	The equipment under test is a class III Handheld thermography camera with laser function for distance measurement, which contains SELV circuit only and powered by building-in lithium battery pack and 5 V d.c. through Micro USB port. Lithium battery pack is powered by external power station or micro USB port in unit.
Material of enclosure	Plastic enclosure & glass for panel.
Other features	Indoor and outdoor used.

**Description of model differences:**

**All models are identical except model designation, lens used and software used.**

**Model list:**

DS-2TP31-03AUF	DS-2TPH16-3AUF	DS-2TP31-3HUF	DS-2TP21-6VFW
DS-2TPH16-6VFW	DS-2TP26-25VFW	DS-2TPH66-25VFW	DS-2TP16-25VFW
DS-2TPH68-25VFW	DS-2TP31-3AUF	DS-2TP31-4AUF	DS-2TP31-5AUF
DS-2TP31-6AUF	DS-2TP31-7AUF	DS-2TP31-8AUF	DS-2TP31-10AUF
DS-2TP33-3AUF	DS-2TP33-4AUF	DS-2TP33-5AUF	DS-2TP33-6AUF
DS-2TP33-7AUF	DS-2TP33-8AUF	DS-2TP33-10AUF	DS-2TP36-3AUF
DS-2TP36-4AUF	DS-2TP36-5AUF	DS-2TP36-6AUF	DS-2TP36-7AUF
DS-2TP36-8AUF	DS-2TP36-10AUF	DS-2TP31-3HUF	DS-2TP31-4HUF
DS-2TP31-5HUF	DS-2TP31-6HUF	DS-2TP31-7HUF	DS-2TP31-8HUF
DS-2TP31-10HUF	DS-2TP33-3HUF	DS-2TP33-4HUF	DS-2TP33-5HUF
DS-2TP33-6HUF	DS-2TP33-7HUF	DS-2TP33-8HUF	DS-2TP33-10HUF
DS-2TP36-3HUF	DS-2TP36-4HUF	DS-2TP36-5HUF	DS-2TP36-6HUF
DS-2TP36-7HUF	DS-2TP36-8HUF	DS-2TP36-10HUF	DS-2TP31-3AXF
DS-2TP31-4AXF	DS-2TP31-5AXF	DS-2TP31-6AXF	DS-2TP31-7AXF
DS-2TP31-8AXF	DS-2TP31-10AXF	DS-2TP33-3AXF	DS-2TP33-4AXF
DS-2TP33-5AXF	DS-2TP33-6AXF	DS-2TP33-7AXF	DS-2TP33-8AXF
DS-2TP33-10AXF	DS-2TP36-3AXF	DS-2TP36-4AXF	DS-2TP36-5AXF
DS-2TP36-6AXF	DS-2TP36-7AXF	DS-2TP36-8AXF	DS-2TP36-10AXF
DS-2TP31-3HXF	DS-2TP31-4HXF	DS-2TP31-5HXF	DS-2TP31-6HXF
DS-2TP31-7HXF	DS-2TP31-8HXF	DS-2TP31-10HXF	DS-2TP33-3HXF
DS-2TP33-4HXF	DS-2TP33-5HXF	DS-2TP33-6HXF	DS-2TP33-7HXF
DS-2TP33-8HXF	DS-2TP33-10HXF	DS-2TP36-3HXF	DS-2TP36-4HXF
DS-2TP36-5HXF	DS-2TP36-6HXF	DS-2TP36-7HXF	DS-2TP36-8HXF
DS-2TP36-10HXF	DS-2TPH10-3AUF	DS-2TPH10-4AUF	DS-2TPH10-5AUF
DS-2TPH10-6AUF	DS-2TPH10-7AUF	DS-2TPH10-8AUF	DS-2TPH10-10AUF
DS-2TPH11-3AUF	DS-2TPH11-4AUF	DS-2TPH11-5AUF	DS-2TPH11-6AUF
DS-2TPH11-7AUF	DS-2TPH11-8AUF	DS-2TPH11-10AUF	DS-2TPH13-3AUF
DS-2TPH13-4AUF	DS-2TPH13-5AUF	DS-2TPH13-6AUF	DS-2TPH13-7AUF
DS-2TPH13-8AUF	DS-2TPH13-10AUF	DS-2TPH10-3HUF	DS-2TPH10-4HUF
DS-2TPH10-5HUF	DS-2TPH10-6HUF	DS-2TPH10-7HUF	DS-2TPH10-8HUF
DS-2TPH10-10HUF	DS-2TPH11-3HUF	DS-2TPH11-4HUF	DS-2TPH11-5HUF
DS-2TPH11-6HUF	DS-2TPH11-7HUF	DS-2TPH11-8HUF	DS-2TPH11-10HUF
DS-2TPH13-3HUF	DS-2TPH13-4HUF	DS-2TPH13-5HUF	DS-2TPH13-6HUF
DS-2TPH13-7HUF	DS-2TPH13-8HUF	DS-2TPH13-10HUF	DS-2TPH10-3AXF
DS-2TPH10-4AXF	DS-2TPH10-5AXF	DS-2TPH10-6AXF	DS-2TPH10-7AXF
DS-2TPH10-8AXF	DS-2TPH10-10AXF	DS-2TPH11-3AXF	DS-2TPH11-3AXF
DS-2TPH11-4AXF	DS-2TPH11-5AXF	DS-2TPH11-6AXF	DS-2TPH11-7AXF
DS-2TPH11-8AXF	DS-2TPH11-10AXF	DS-2TPH13-3AXF	DS-2TPH13-4AXF
DS-2TPH13-5AXF	DS-2TPH13-6AXF	DS-2TPH13-7AXF	DS-2TPH13-8AXF
DS-2TPH13-10AXF	DS-2TPH10-3HXF	DS-2TPH10-4HXF	DS-2TPH10-5HXF
DS-2TPH10-6HXF	DS-2TPH10-7HXF	DS-2TPH10-8HXF	DS-2TPH10-10HXF
DS-2TPH11-3HXF	DS-2TPH11-4HXF	DS-2TPH11-5HXF	DS-2TPH11-6HXF
DS-2TPH11-7HXF	DS-2TPH11-8HXF	DS-2TPH11-10HXF	DS-2TPH13-3HXF
DS-2TPH13-4HXF	DS-2TPH13-5HXF	DS-2TPH13-6HXF	DS-2TPH13-7HXF
DS-2TPH13-8HXF	DS-2TPH13-10HXF	DS-2TPH30-3AUF	DS-2TPH30-4AUF
DS-2TPH30-5AUF	DS-2TPH30-6AUF	DS-2TPH30-7AUF	DS-2TPH30-8AUF
DS-2TPH30-10AUF	DS-2TPH31-3AUF	DS-2TPH31-4AUF	DS-2TPH31-5AUF
DS-2TPH31-6AUF	DS-2TPH31-7AUF	DS-2TPH31-8AUF	DS-2TPH31-10AUF
DS-2TPH33-3AUF	DS-2TPH33-4AUF	DS-2TPH33-5AUF	DS-2TPH33-6AUF
DS-2TPH33-7AUF	DS-2TPH33-8AUF	DS-2TPH33-10AUF	DS-2TPH30-3HUF
DS-2TPH30-4HUF	DS-2TPH30-5HUF	DS-2TPH30-6HUF	DS-2TPH30-7HUF
DS-2TPH30-8HUF	DS-2TPH30-10HUF	DS-2TPH31-3HUF	DS-2TPH31-4HUF
DS-2TPH31-5HUF	DS-2TPH31-6HUF	DS-2TPH31-7HUF	DS-2TPH31-8HUF
DS-2TPH31-10HUF	DS-2TPH33-3HUF	DS-2TPH33-4HUF	DS-2TPH33-5HUF
DS-2TPH33-6HUF	DS-2TPH33-7HUF	DS-2TPH33-8HUF	DS-2TPH33-10HUF
DS-2TPH30-3AXF	DS-2TPH30-4AXF	DS-2TPH30-5AXF	DS-2TPH30-6AXF
DS-2TPH30-7AXF	DS-2TPH30-8AXF	DS-2TPH30-10AXF	DS-2TPH31-3AXF

DS-2TPH31-4AXF	DS-2TPH31-5AXF	DS-2TPH31-6AXF	DS-2TPH31-7AXF
DS-2TPH31-8AXF	DS-2TPH31-10AXF	DS-2TPH33-3AXF	DS-2TPH33-4AXF
DS-2TPH33-5AXF	DS-2TPH33-6AXF	DS-2TPH33-7AXF	DS-2TPH33-8AXF
DS-2TPH33-10AXF	DS-2TPH30-3HXF	DS-2TPH30-4HXF	DS-2TPH30-5HXF
DS-2TPH30-6HXF	DS-2TPH30-7HXF	DS-2TPH30-8HXF	DS-2TPH30-10HXF
DS-2TPH31-3HXF	DS-2TPH31-4HXF	DS-2TPH31-5HXF	DS-2TPH31-6HXF
DS-2TPH31-7HXF	DS-2TPH31-8HXF	DS-2TPH31-10HXF	DS-2TPH33-3HXF
DS-2TPH33-4HXF	DS-2TPH33-5HXF	DS-2TPH33-6HXF	DS-2TPH33-7HXF
DS-2TPH33-8HXF	DS-2TPH33-10HXF	-	-


**Description of special features:**

(HV circuits, high pressure systems etc.)

N/A



IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
<b>4</b>	<b>TESTS</b>		P
4.4	Testing in SINGLE FAULT CONDITIONS		P
4.4.1	Fault tests	(see Form A.1)	P
4.4.2	Application of SINGLE FAULT CONDITIONS		P
4.4.2.1	SINGLE FAULT CONDITIONS not covered by 4.4.2.2 to 4.4.2.14	(see Form A.1)	P
4.4.2.2	PROTECTIVE IMPEDANCE		N/A
4.4.2.3	PROTECTIVE CONDUCTOR	(see Form A.6)	N/A
4.4.2.4	Equipment or parts for short-term or intermittent operation		N/A
4.4.2.5	Motors		—
	– stopped while fully energized		N/A
	– prevented from starting		N/A
	– one phase interrupted (multi-phase)		N/A
4.4.2.6	Capacitors		N/A
4.4.2.7	MAINS transformers		N/A
4.4.2.7.2	Short circuit	(see Form A.39)	N/A
4.4.2.7.3	Overload	(see Forms A.26B and A.40)	N/A
4.4.2.8	Outputs		P
4.4.2.9	Equipment for more than one supply		N/A
4.4.2.10	Cooling	(see Form A.26A)	—
	– air holes closed		N/A
	– fans stopped		N/A
	– coolant stopped		N/A
	– loss of cooling liquid		N/A
4.4.2.11	Heating devices		—
	– timer overridden		N/A
	– temperature controller overridden		N/A
4.4.2.12	Insulation between circuits and parts		N/A
4.4.2.13	Interlocks		N/A
4.4.2.14	Voltage selectors		N/A
4.4.3	Duration of tests	(see Form A.1)	—
4.4.4	Conformity after application of fault conditions	(see Forms A.1, A.6 and A.18)	P
<b>5</b>	<b>MARKING AND DOCUMENTATION</b>		P
<b>5.1</b>	<b>Marking</b>		P
5.1.1	General		P
	Required equipment markings		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Visible from the exterior; or		P
	– Visible after removing cover or opening door		N/A
	– Visible after removal from a rack or panel		N/A
	Not put on parts which can be removed by an operator		P
	Letter symbols (IEC 60027) used		P
	Graphic symbols of Table 1 used		P
5.1.2	Identification		P
	Equipment is identified by:		—
	a) Manufacturer's or supplier's name or trademark		P
	b) Model number, name or other means		P
	Manufacturing location identified	Only one factory	N/A
5.1.3	MAINS supply	EUT was powered by battery and external DC power source through USB port, Not connect to mains.	N/A
	Equipment is marked as follows:		—
	a) Nature of supply:		—
	1) a.c. RATED MAINS frequency or range of frequencies .....		—
	2) d.c. with symbol 1.....	The DC symbol  (IEC 60417-5031 (2002-10)) was used.	—
	b) RATED supply voltage(s) or range .....		—
	c) Max. RATED power (W or VA) or input current .....		—
	The marked value not less than 90 % of the maximum value	(see Form A.2)	N/A
	If more than one voltage range:		—
	Separate values marked; or		N/A
	Values differ by less than 20 %	(see Form A.2)	N/A
	d) OPERATOR-set for different RATED supply voltages:		—
	Indicates the equipment set voltage		N/A
	PORTABLE EQUIPMENT indication is visible from the exterior		N/A
	Changing the setting changes the indication		N/A
	e) Accessory MAINS socket-outlets accepting standard MAINS plugs are marked:		—
	With the voltage if it is different from the MAINS supply voltage.....		—
	For use only with specific equipment		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	If not marked for specific equipment it is marked with:		—
	The maximum RATED current or power; or		N/A
	Symbol 14 with full details in the documentation		N/A
5.1.4	Fuses		N/A
	OPERATOR replaceable fuse marking (see also 5.4.5).....:		—
5.1.5	TERMINALS, connections and operating devices		P
5.1.5.1	General		P
	Where necessary for safety, indication of purpose of TERMINALS, connectors, controls and indicators marked	Laser marking was considered.	P
	If insufficient space, symbol 14 used		N/A
	Push-buttons and actuators of emergency stop devices and indicators:		—
	– used only to indicate a warning of danger; or		N/A
	– the need for urgent action		N/A
	– coloured red		N/A
	– coded as specified in IEC 60073		N/A
	Supplementary means of coding provided, if meaning of colour relates (see IEC 60073):		—
	– to safety of persons; or		N/A
	– safety of the environment		N/A
5.1.5.2	TERMINALS		—
	MAINS supply TERMINAL identified		N/A
	Other TERMINAL marking:		—
	a) FUNCTIONAL EARTH TERMINALS marked with symbol 5		N/A
	b) PROTECTIVE CONDUCTOR TERMINALS:		—
	Symbol 6 is placed close to or on the TERMINAL; or		N/A
	Part of appliance inlet		N/A
	c) TERMINALS of circuits (symbol 7 used)		N/A
	d) HAZARDOUS LIVE TERMINALS supplied from the interior		N/A
	Standard MAINS socket outlet used; or		N/A
	RATINGS marked; or		N/A
	Symbol 14 used		N/A
5.1.6	Switches and circuit-breakers		N/A
	If disconnecting device, off position clearly marked		N/A
	If push-button used as power supply switch:		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Symbol 9 and 15 used for on-position		N/A
	– Symbol 10 and 16 used for off-position		N/A
	– Pair of symbols 9, 15 and 10, 16 close together		N/A
5.1.7	Equipment protected by DOUBLE INSULATION or REINFORCED INSULATION		N/A
	Protected throughout (symbol 11 used)		N/A
	Only partially protected (symbol 11 not used)		N/A
5.1.8	Field-wiring TERMINAL boxes		N/A
	If TERMINAL or ENCLOSURE exceeds 60 °C:	(see Form A.26A)	—
	Cable temperature RATING marked .....		—
	Marking visible before and during connection or beside TERMINAL		N/A
<b>5.2</b>	<b>Warning markings</b>		P
	Visible when ready for NORMAL USE		P
	Are near or on applicable parts		P
	Symbols and text correct dimensions and colour:		—
	a) Symbols min 2,75 mm and text 1,5 mm high and contrasting in colour with background		P
	b) Symbols and text moulded, stamped or engraved in material min. 2,0 mm high and		N/A
	0,5 mm depth or raised if not contrasting in colour		N/A
	If necessary marked with symbol 14, or		N/A
	Additional symbols such as symbol 12, 13 or 17 used to indicate the nature of HAZARD		N/A
	Statement to place equipment in a safe state before access by using a tool to HAZARDOUS parts is permitted		N/A
<b>5.3</b>	<b>Durability of markings</b>		P
	The required markings remain clear and legible in NORMAL USE	(see Form A.3)	P
<b>5.4</b>	<b>Documentation</b>		P
5.4.1	General		P
	Equipment is accompanied by documentation for safety purposes for OPERATOR or RESPONSIBLE BODY		P
	Safety documentation for service personnel authorized by the manufacturer		P
	Documentation necessary for safe operation is provided in printed media or		P
	in electronic media if available at any time		N/A
	Documentation includes:		—
	a) Intended use		P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) Technical specification		P
	c) Name and address of manufacturer or supplier		P
	d) Information specified in 5.4.2 to 5.4.6		P
	e) Information to mitigate residual RISK (see also subclause 17)		N/A
	f) Accessories for safe operation of the equipment specified		N/A
	g) Guidance provided to check correct function of the equipment, if incorrect reading may cause a HAZARD from harmful or corrosive substances of HAZARDOUS live parts		N/A
	h) Instructions for lifting and carrying		N/A
	Warning statements and a clear explanation of warning symbols:		—
	– provided in the documentation; or		N/A
	– information is marked on the equipment		N/A
5.4.2	Equipment RATINGS		P
	Documentation includes:		—
	a) Supply voltage or voltage range..... : 5 Vd.c.		—
	Frequency or frequency range ..... : Powered by DC		—
	Power or current rating..... : 1,1 A, 5,5W		—
	b) Description of all input and output connections in accordance to 6.6.1 a)		P
	c) RATING of insulation of external circuits in accordance to 6.6.1 b)		N/A
	d) Statement of the range of environmental conditions (refer to 1.4):		—
	1) indoor or outdoor use,		P
	2) altitude,		P
	3) temperature,		P
	4) relative humidity,		P
	5) MAINS supply voltage fluctuations,		N/A
	6) OVERVOLTAGE CATEGORY,		N/A
	7) WET LOCATION, if applicable,		N/A
	8) POLLUTION DEGREE of the intended environment		N/A
	e) Degree of ingress protection (IEC 60529)		N/A
	f) If impact rating less than 5 J:		—
	IK code in accordance to IEC 62262 marked; or		N/A
	symbol 14 of Table 1 marked, with		N/A
	RATED energy level and test method stated		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
5.4.3	Equipment installation		P
	Documentation includes instructions for:		—
	a) Assembly, location and mounting requirements		P
	b) Instructions for protective earthing		N/A
	c) Connections to supply		P
	d) PERMANENTLY CONNECTED EQUIPMENT:		—
	1) Supply wiring requirements		N/A
	2) If external switch or circuit-breaker, requirements and location recommendation		N/A
	e) Ventilation requirements		N/A
	f) Safety characteristics for special external services (e. g. maximum and minimum temperature, pressure, flow of air, cooling liquid)		N/A
	g) Instructions relating to sound level		N/A
5.4.4	Equipment operation		P
	Instructions for use include:		—
	a) Identification and description of operating controls		P
	b) Positioning for disconnection		N/A
	c) Instructions for interconnection to accessories or other equipment		P
	d) Specification of intermittent operation limits		N/A
	e) Explanation of symbols used		P
	f) Replacement of consumable materials		P
	g) Cleaning and decontamination		P
	h) Listing of any poisonous or injurious gases and quantities		N/A
	i) RISK reduction procedures relating to flammable liquids (see 9.5 c)		N/A
	j) RISK reduction procedures relating burn from surfaces permitted to exceed limits of 10.1		N/A
	Additional precautions for IEC 60950 conforming equipment in regard to moistures and liquids		P
	A statement about protection impairment if used in a manner not specified by the manufacturer		P
5.4.5	Equipment maintenance and service		P
	Instructions for RESPONSIBLE BODY include:	See follow	—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Instructions sufficient in detail permitting safe maintenance and inspection and continued safety:	Sufficient detail to permit safe maintenance, inspection and testing of the equipment, and to ensure continued safety of the equipment after the maintenance inspection and test procedure	—
	Instruction against the use of detachable MAINS supply cord with inadequate RATING		N/A
	Specific battery type of user replaceable batteries		P
	Any manufacturer specified parts		P
	RATING and characteristics of fuses		N/A
	Instructions include following subjects permitting safe servicing and continued safety:		—
	a) Product specific RISKS may affect service personnel	Laser class 2 source and battery were considered.	P
	b) Protective measures for these RISKS	Warning marking used for laser.	P
	c) Verification of the safe state after repair		P
5.4.6	Integration into systems or effects resulting from special conditions		N/A
	Aspects described in documentation		N/A

<b>6</b>	<b>PROTECTION AGAINST ELECTRIC SHOCK</b>		P
<b>6.1</b>	<b>General</b>	(see Forms A.14 and A.15)	P
6.1.1	Requirements		P
	Protection against electric shock maintained in NORMAL CONDITION and SINGLE FAULT CONDITION	EUT was powered by building-in 3,6Vdc lithium battery pack and 5Vdc power source.no boosted hazardous circuits exist.	N/A
	ACCESSIBLE parts not HAZARDOUS LIVE		P
	Voltage, current, charge or energy below the limits in NORMAL CONDITION and in SINGLE FAULT CONDITION between:		—
	ACCESSIBLE parts and earth		N/A
	two ACCESSIBLE parts on same piece of the equipment within a distance of 1,8 m		N/A
	Conformity is checked by the determination of 6.2 and 6.3 followed by the tests of 6.4 to 6.11		N/A
6.1.2	Exceptions		N/A
	Following HAZARDOUS LIVE parts may be ACCESSIBLE to an OPERATOR:		—
	a) parts of lamps and lamp sockets after lamp removal		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) parts to be replaced by OPERATOR only by the use of tool and warning marking		N/A
	Those parts not HAZARDOUS LIVE 10 s after interruption of supply	(see Form A.5 )	N/A
	Capacitance test if charge is received from internal capacitor	(see Forms A.4 and A.5)	N/A
<b>6.2</b>	<b>Determination of ACCESSIBLE parts</b>	(see Form A.4)	P
6.2.1	General		P
	Unless obviously determination of ACCESSIBLE parts as specified in 6.2.2 to 6.2.4		P
6.2.2	Examination		P
	– with jointed test finger (as specified B.2)		P
	– with rigid test finger (as specified B.1) and a force of 10 N		N/A
6.2.3	Openings above parts that are HAZARDOUS LIVE		N/A
	– test pin with length of 100 mm and 4 mm in diameter applied		N/A
6.2.4	Openings for pre-set controls		N/A
	– test pin with length of 100 mm and 3 mm in diameter applied		N/A
<b>6.3</b>	<b>Limit values for ACCESSIBLE parts</b>		P
6.3.1	Levels in NORMAL CONDITION	(see Form A.5)	P
	a) Voltage limits less than 30 V r.m.s. and 42,4 V peak or 60 V d.c.		P
	for WET LOCATIONS voltage limits less than 16 V r.m.s. and 22,6 V peak or 35 V d.c.		N/A
	Voltages are not HAZARDOUS LIVE the levels of:		—
	b) Current less than 0,5 mA r.m.s. for sinusoidal, 0,7 mA peak non-sinusoidal or mixed frequencies or 2 mA d.c. when measured with measuring circuit A.1 or A.2 if less than 100 Hz		N/A
	for WET LOCATIONS measuring circuit A.4 used		N/A
	70 mA r.m.s. when measured with circuit A.3 for higher frequencies		N/A
	c) Levels of capacitive charge or energy less:		—
	1) 45 $\mu$ C for voltages up to 15 kV peak or d.c. or line A of Figure 3		N/A
	2) 350 mJ stored energy for voltages above 15 kV peak or d.c.		N/A
6.3.2	Levels in SINGLE FAULT CONDITION	(see Form A.6)	P
	a) Voltage limits less than 50 V r.m.s. and 70 V peak or 120 V d.c.		P



IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	for WET LOCATIONS voltage limits less than 33 V r.m.s. and 46,7 V peak or 70 V d.c.		N/A
	Voltages are not HAZARDOUS LIVE the levels of:		—
	b) Current less than 3,5 mA r.m.s. for sinusoidal, 5 mA peak non-sinusoidal or mixed frequencies or 15 mA d.c. when measured with measuring circuit A.1 or A.2 if less than 100 Hz		N/A
	for WET LOCATIONS measuring circuit A.4 used		N/A
	500 mA r.m.s. when measured with circuit A.3 for higher frequencies		N/A
	c) Levels of capacitive charge or energy less line B of Figure 3		N/A
<b>6.4</b>	<b>Primary means of protection</b>	EUT was powered by building-in 3,6Vdc lithium battery pack and 5Vdc power source.no boosted hazardous circuits exist.	N/A
6.4.1	General		N/A
	ACCESSIBLE parts prevented from being HAZARDOUS LIVE by one or more of following means:		—
	a) ENCLOSURES or PROTECTIVE BARRIERS (see 6.4.2)		N/A
	b) BASIC INSULATION (see 6.4.3)		N/A
	c) Impedance (see 6.4.4)		N/A
6.4.2	ENCLOSURES or PROTECTIVE BARRIERS	(see Forms A.15 and A.16)	N/A
	– meet rigidity requirements of 8.1		N/A
	– meet requirements for BASIC INSULATION, if protection is provided by insulation		N/A
	– meet requirements of 6.7 for CREEPAGE and – CLEARANCES between ACCESSIBLE parts and – HAZARDOUS live parts, if protection is provided by – limited access		N/A
6.4.3	BASIC INSULATION	(see Forms A.15 and A.16)	N/A
	– meet CLEARANCE, CREEPAGE DISTANCE and solid insulation requirements of 6.7		N/A
6.4.4	Impedance	(see Forms A.12 and A.15)	N/A
	Impedance used as primary means of protection meets all the following requirements:		—
	a) limits current or voltage to level of 6.3.2	(see Form A.6)	N/A
	b) RATED for maximum WORKING VOLTAGE and the amount of power it will dissipate		N/A
	c) CLEARANCE, CREEPAGE DISTANCE between terminations of the impedance meet requirements of BASIC INSULATION of 6.7	(see Form A.15)	N/A
<b>6.5</b>	<b>Additional means of protection in case of SINGLE FAULT CONDITION</b>		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
6.5.1	General		N/A
	ACCESSIBLE parts are prevented from becoming HAZARDOUS live by the primary means of protection and supplemented by one of:		—
	a) PROTECTIVE BONDING (see 6.5.2)		N/A
	b) SUPPLEMENTARY INSULATION (see 6.5.3)		N/A
	c) automatic disconnection of the supply (see 6.5.5)		N/A
	d) current- or voltage-limiting device (see 6.5.6)		N/A
	Alternatively one of the single means of protection is used:		—
	e) REINFORCED INSULATION (see 6.5.3)		N/A
	f) PROTECTIVE IMPEDANCE (see 6.5.4)		N/A
6.5.2	PROTECTIVE BONDING	(see Forms A.7, A.8, A.9, A.10 or A.11)	N/A
6.5.2.1	General		N/A
	ACCESSIBLE conductive parts, may become HAZARDOUS LIVE in SINGLE FAULT CONDITION:		—
	Bonded to the PROTECTIVE CONDUCTOR TERMINAL; or		N/A
	Separated by conductive screen or barrier bonded to PROTECTIVE CONDUCTOR TERMINAL		N/A
6.5.2.2	Integrity of PROTECTIVE BONDING		—
	a) PROTECTIVE BONDING consists of directly connected structural parts or discrete conductors or both; and withstands thermal and dynamic stresses		N/A
	b) Soldered connections:		—
	Independently secured against loosening		N/A
	Not used for other purposes		N/A
	c) Screw connections are secured		N/A
	d) PROTECTIVE BONDING not interrupted; or		N/A
	except as removable part that carries MAINS SUPPLY input connection to the whole equipment		N/A
	e) Any movable PROTECTIVE BONDING connection specifically designed, and meets 6.5.2.4		N/A
	f) No external metal braid of cables used (not regarded as PROTECTIVE BONDING)		N/A
	g) IF MAINS SUPPLY passes through:		—
	Means provided for passing protective conductor;		N/A
	Impedance meets 6.5.2.4		N/A
	h) Protective conductors bare or insulated, if insulated, green/yellow		N/A
	Exceptions:		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	1) earthing braids;		N/A
	2) internal protective conductors etc.;		N/A
	Green/yellow not used for other purposes		N/A
	TERMINAL suitable for connection of a PROTECTIVE CONDUCTOR, and meets 6.5.2.3		N/A
6.5.2.3	PROTECTIVE CONDUCTOR TERMINAL		—
	a) Contact surfaces are metal		N/A
	b) Appliance inlet used		N/A
	c) For rewirable cords and PERMANENTLY CONNECTED EQUIPMENT, PROTECTIVE CONDUCTOR TERMINAL is close to MAINS supply TERMINALS		N/A
	d) If no MAINS supply is required, any PROTECTIVE CONDUCTOR TERMINAL:		—
	Is near terminals of circuit for which protective earthing is necessary		N/A
	External if other terminals external		N/A
	e) Equivalent current-carrying capacity to MAINS supply TERMINALS	(see Form A.7)	N/A
	f) If plug-in, makes first and breaks last		N/A
	g) If also used for other bonding purposes, PROTECTIVE CONDUCTOR:		—
	Applied first;		N/A
	Secured independently;		N/A
	Unlikely to be removed by servicing		N/A
	h) PROTECTIVE CONDUCTOR of measuring circuit:		—
	1) Current RATING equivalent to measuring circuit TERMINAL;		N/A
	2) PROTECTIVE BONDING: not interrupted by any switch or interrupting device		N/A
	i) FUNCTIONAL EARTH TERMINALS allow independent connection		N/A
	j) If a binding screw used for PROTECTIVE CONDUCTOR TERMINAL:		—
	Suitable size for bond wire		N/A
	Not smaller than M 4		N/A
	At least 3 turns of screw engaged		N/A
	Passes tightening torque test	(see Form A.8)	N/A
	k) Contact pressure not capable being reduced by deformation of materials		N/A
6.5.2.4	Impedance of PROTECTIVE BONDING of plug-connected equipment	(see Form A.9)	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Impedance between PROTECTIVE CONDUCTOR TERMINAL and each ACCESSIBLE part where PROTECTIVE BONDING is specified, is:		—
	– less than 0,1 Ohm; or		N/A
	– less than 0,2 Ohm if equipment is provided with non-detachable cord		N/A
6.5.2.5	Impedance of PROTECTIVE BONDING of PERMANENTLY CONNECTED EQUIPMENT	(see Form A.10)	N/A
6.5.2.6	Transformer PROTECTIVE BONDING screen	(see Form A.11)	N/A
	Transformer provided with screen for PROTECTIVE BONDING:		—
	screen bonding consists of directly connected structural parts or discrete conductors or both; and withstands thermal and dynamic stresses (see 6.5.2.2 a )		N/A
	screen bonding with soldered connection (see 6.5.2.2 b ) is:		—
	– Independently secured against loosening		N/A
	– Not used for other purposes		N/A
6.5.3	SUPPLEMENTARY and REINFORCED INSULATION		N/A
	Meet CLEARANCE, CREEPAGE DISTANCE and solid insulation requirements of 6.7		N/A
6.5.4	PROTECTIVE IMPEDANCE	(see Form A.12)	N/A
	Limits current or voltage to level of 6.3.1 in NORMAL and to level of 6.3.2 in SINGLE FAULT CONDITION		N/A
	CLEARANCE, CREEPAGE DISTANCE between terminations of the impedance meet requirements of DOUBLE or REINFORCED INSULATION of 6.7	(see Form A.15)	N/A
	The PROTECTIVE IMPEDANCE consists of one or more of the following:	(see TABLE 1.A and Form A.12)	—
	a) appropriate single component suitable for safety and reliability for protection, it is:		—
	1) RATED twice the maximum WORKING VOLTAGE		N/A
	2) resistor RATED for twice the power dissipation for maximum WORKING VOLTAGE		N/A
	b) combination of components		N/A
	Single electronic device not used as PROTECTIVE IMPEDANCE		N/A
6.5.5	Automatic disconnection of the supply		N/A
	a) RATED to disconnect the load within time specified in Figure 2		N/A
	b) RATED for the maximum load conditions of the equipment		N/A
6.5.6	Current- or voltage-limiting devices	(see Form A.13)	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Device complies with all of:		—
	a) RATED to limit the current or voltage to the level of 6.3.2	(see Form A.6)	N/A
	b) RATED for the maximum WORKING VOLTAGE; and		N/A
	RATED for the maximum operational current if applicable		N/A
	c) CLEARANCE, CREEPAGE DISTANCE between terminations of the impedance meet requirements of SUPPLEMENTARY INSULATION of 6.7	(see Forms A.14 and A.15)	N/A
<b>6.6</b>	<b>Connections to external circuits</b>		P
6.6.1	General		P
	Connections do not cause ACCESSIBLE parts of the following to become HAZARDOUS LIVE in NORMAL CONDITION or SINGLE FAULT CONDITION:		—
	– the external circuits		P
	– the equipment		P
	Protection achieved by separation of circuits; or		N/A
	short circuit of separation does not cause a HAZARD		N/A
	Instructions or markings for each terminal include:		—
	a) RATED conditions for TERMINAL		N/A
	b) Required RATING of external circuit insulation		N/A
6.6.2	TERMINALS for external circuits		N/A
	TERMINALS which receive a charge from an internal capacitor are not HAZARDOUS LIVE after 10 s of interrupting supply connection	(see Form A.5)	N/A
6.6.3	Circuits with terminals which are HAZARDOUS LIVE		N/A
	These circuits are:		—
	Not connected to ACCESSIBLE conductive parts; or		N/A
	Connected to ACCESSIBLE conductive parts, but are not MAINS CIRCUITS and have one TERMINAL contact at earth potential		N/A
	No ACCESSIBLE conductive parts are HAZARDOUS LIVE		N/A
6.6.4	Terminals for stranded conductors		N/A
	No RISK of accidental contact because:		—
	– Located or shielded		N/A
	– Self-evident or marked whether or not connected to ACCESSIBLE conductive parts		N/A
	Complies as applicable:		—
	a) Manufacturer's specified maximum length of removed insulation, or		N/A
	b) 8 mm length of insulation removed		N/A
<b>6.7</b>	<b>Insulation requirements</b>	(see Form A.14)	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
6.7.1	The nature of insulation		N/A
6.7.1.1	General		N/A
	Insulation between ACCESSIBLE parts or between separate circuits consist of CLEARANCES, CREEPAGE DISTANCES and solid insulation if provided as protection against a HAZARD		N/A
6.7.1.2	CLEARANCES		N/A
	Required CLEARANCES reflecting factors of 6.7.1.1	(see Forms A.14 and A.15)	N/A
	Equipment rated for operating altitude greater than 2000 m correction factor of Table 3 of 61010-1 applied		N/A
6.7.1.3	CREEPAGE DISTANCES		N/A
	Required CREEPAGE DISTANCES reflecting factors of 6.7.1.1 a) to d)	(see Forms A.14 and A.15)	N/A
	CTI material group reflected by requirements		N/A
	CTI test performed		N/A
6.7.1.4	Solid insulation		N/A
	Required solid insulation reflecting factors of 6.7.1.1 a) to d)	(see Forms A.14 and A.15)	N/A
6.7.1.5	Requirements for insulation according to type of circuit	(see Forms A.14 and A.15)	N/A
	a) 6.7.2 MAINS circuits of OVERVOLTAGE CATEGORY II up to nominal supply voltage of 300 V		N/A
	b) 6.7.3 secondary circuits separated from circuits defined in a) by transformer		N/A
	c) K.1 MAINS circuits of OVERVOLTAGE CATEGORY III and IV or OVERVOLTAGE CATEGORY II over 300 V		N/A
	d) K.2 secondary circuits separated from circuits defined in c) by transformer		N/A
	e) K.3 circuits having one or more of:		—
	1) maximum TRANSIENT OVERVOLTAGE is limited to known level below the level of MAINS CIRCUIT		N/A
	2) maximum TRANSIENT OVERVOLTAGE above the level of MAINS CIRCUIT		N/A
	3) WORKING VOLTAGE is the sum of more than one circuit or a mixed voltage		N/A
	4) WORKING VOLTAGE includes recurring peak voltage, may include non-sinusoidal or non-periodic waveform		N/A
	5) WORKING VOLTAGE with a frequency above 30 kHz		N/A
6.7.2	Insulation for MAINS CIRCUITS of OVERVOLTAGE CATEGORY II with a nominal supply voltage up to 300 V		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
6.7.2.1	CLEARANCES and CREEPAGE DISTANCES	(see Forms A.14 and A.15)	—
	Values for MAINS CIRCUITS of Table 4 are met		N/A
	Coatings to achieve reduction to POLLUTION DEGREE 1 comply with requirements of Annex H		N/A
6.7.2.2	Solid insulation		N/A
6.7.2.2.1	General		N/A
	Withstands electrical and mechanical stresses in normal use and all RATED environmental conditions of 1.4		N/A
	Equipment passed voltage tests of 6.8.3 with values of Table 5	(see Form A.18)	N/A
	Complies as applicable:		—
	a) ENCLOSURE or PROTECTIVE BARRIER of Clause 8		N/A
	b) moulded and potted parts requirements of 6.7.2.2.2		N/A
	c) inner layers of printed wiring boards requirements of 6.7.2.2.3		N/A
	d) thin-film insulation requirements of 6.7.2.2.4		N/A
6.7.2.2.2	Moulded and potted parts		—
	Conductors between same two layers are separated by at least 0,4 mm after moulding is completed		N/A
6.7.2.2.3	Inner insulating layers of printed wiring boards		—
	Separated by at least 0,4 mm between same two layers		N/A
	REINFORCED INSULATION have adequate electric strength; one of following methods used:		—
	a) thickness of insulation is at least 0,4 mm		N/A
	b) insulation is assembled of minimum two separate layers, each RATED for test voltage of Table 5 for BASIC INSULATION		N/A
	c) insulation is assembled of minimum two separate layers, where the combination is rated for test voltage of Table 5 for REINFORCED INSULATION		N/A
6.7.2.2.4	Thin-film insulation		—
	Conductors between same two layers are separated by applicable CLEARANCES and CREEPAGE DISTANCE of 6.7.2.1		N/A
	REINFORCED INSULATION have adequate electric strength; one of the following methods used:		—
	a) thickness through the insulation at least 0,4 mm		N/A
	b) insulation is assembled of min. two separate layers, each RATED for test voltage of Table 5 for BASIC INSULATION	(see Form A.18)	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) insulation is assembled of min. three separate layers, where the combination of two layers passed voltage tests of 6.8.3 with values of Table 5 for REINFORCED INSULATION	(see Form A.18)	N/A
6.7.3	Insulation for secondary circuits derived from MAINS CIRCUITS of OVERVOLTAGE CATEGORY II up to 300 V		N/A
6.7.3.1	General		N/A
	Secondary circuits where separation from MAINS CIRCUITS is achieved by a transformer providing:		—
	– REINFORCED INSULATION		N/A
	– DOUBLE INSULATION		N/A
	– screen connected to the PROTECTIVE CONDUCTOR TERMINAL		N/A
6.7.3.2	CLEARANCES	(see Forms A.14 and A.15)	N/A
	a) meet the values of Table 6 for BASIC INSULATION and SUPPLEMENTARY INSULATION; or		N/A
	twice the values of Table 6 for REINFORCED INSULATION; or		N/A
	b) pass the voltage tests of 6.8 with values of Table 6;	(see Form A.18)	N/A
	with following adjustments:		—
	1) values for reinforced insulation are 1,6 times the values for basic insulation		N/A
	2) if operating altitude is greater than 2000 m values of CLEARANCES multiplied with factor of Table 3		N/A
	3) minimum CLEARANCE is 0,2 mm for POLLUTION DEGREE 2 and 0,8 mm for POLLUTION DEGREE 3		N/A
6.7.3.3	CREEPAGE DISTANCES	(see Forms A.14 and A.15)	N/A
	Based on WORKING VOLTAGE meets the values of Table 7 for BASIC and SUPPLEMENTARY INSULATION		N/A
	Values for REINFORCED INSULATION are twice the values of BASIC INSULATION		N/A
	Coatings to achieve reduction to POLLUTION DEGREE 1 comply with requirements of Annex H		N/A
6.7.3.4	Solid insulation		N/A
6.7.3.4.1	General		N/A
	Withstands electrical and mechanical stresses in normal use and all RATED environmental conditions of 1.4		—
	a) Equipment passed voltage test of 6.8.3.1 for 5 s with VALUES of Table 6 for BASIC and SUPPLEMENTARY INSULATION	(see Form A.18)	N/A
	values for REINFORCED INSULATION are 1,6 times the values of BASIC INSULATION		N/A



IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) if WORKING VOLTAGE exceeds 300 V, equipment passed voltage test of 6.8.3.1 for 1 min with a test voltage of 1,5 times working voltage for BASIC or SUPPLEMENTARY INSULATION	(see Form A.18)	N/A
	value for REINFORCED INSULATION are twice the WORKING VOLTAGE		N/A
	Complies as applicable:		—
	1) ENCLOSURE or PROTECTIVE BARRIER of Clause 8		N/A
	2) moulded and potted parts requirements of 6.7.3.4.2		N/A
	3) inner layers of printed wiring boards requirements of 6.7.3.4.3		N/A
	4) thin-film insulation requirements of 6.7.3.4.4		N/A
6.7.3.4.2	Moulded and potted parts		—
	Conductors between same two layers are separated by applicable distances of Table 8		N/A
6.7.3.4.3	Inner insulation layers of printed wiring boards		—
	Separated by at least the applicable distances of Table 8 between same two layers		N/A
	REINFORCED INSULATION have adequate electric strength; one of following methods used:		—
	a) thickness at least applicable distance of Table 8		N/A
	b) insulation is assembled of minimum two separate layers, each RATED for test voltage of Table 6 for BASIC INSULATION	(see Form A.18)	N/A
	c) insulation is assembled of min. two separate layers, where the combination is RATED for 1,6 times the test voltage of Table 6	(see Form A.18)	N/A
6.7.3.4.4	Thin-film insulation		—
	Conductors between same two layers are separated by applicable CLEARANCES and CREEPAGE DISTANCE of 6.7.3.2 and 6.7.3.3		N/A
	REINFORCED INSULATION have adequate electric strength; one of following methods used:		—
	a) thickness at least applicable distance of Table 8		N/A
	b) insulation is assembled of min. two separate layers, each RATED for test voltage of Table 6 for BASIC INSULATION	(see Form A.18)	N/A
	c) insulation is assembled of min. three separate layers, where the combination of two layers passed voltage tests with 1,6 time values of Table 6:	(see Form A.18)	—
	a.c. test of 6.8.3.1; or		N/A
	d.c. test of 6.8.3.2 for circuits stressed only by d.c. voltages		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
<b>6.8</b>	<b>Procedure for voltage tests</b>	(see Forms A.14 and A.18)	N/A
<b>6.9</b>	<b>Constructional requirements for protection against electric shock</b>		N/A
6.9.1	General		N/A
	If a failure could cause a HAZARD:		—
	a) security of wiring connections		N/A
	b) screws securing removable covers		N/A
	c) accidental loosening		N/A
	d) CLEARANCES and CREEPAGE DISTANCES not reduced below the values of basic insulation by loosening of parts or wires		N/A
6.9.2	Insulating materials		N/A
	Material not to be used for safety relevant insulation:		—
	a) easily damaged materials not used		N/A
	b) non-impregnated hygroscopic materials not used		N/A
6.9.3	Colour coding		N/A
	Green-and-yellow insulation shall not be used except:		—
	a) protective earth conductors;		N/A
	b) PROTECTIVE BONDING conductors;		N/A
	c) potential equalization conductors;		N/A
	d) functional earth conductors		N/A
<b>6.10</b>	<b>Connection to MAINS supply source and connections between parts of equipment</b>		N/A
6.10.1	MAINS supply cords		N/A
	RATED for maximum equipment current (see 5.1.3 c)		N/A
	Cable complies with IEC 60227 or IEC 60245		N/A
	Heat-resistant if likely to contact hot parts		N/A
	Temperature RATING (cord and inlet) .....		—
	Green/yellow used only for connection to PROTECTIVE CONDUCTOR TERMINALS		N/A
	Detachable cords with IEC 60320 MAINS connectors:		—
	Conform to IEC 60799; or		N/A
	Have the current RATING of the MAINS connector		N/A
6.10.2	Fitting of non-detachable MAINS supply cords		N/A
6.10.2.1	Cord entry		—
	a) inlet or bushing with a smoothly rounded opening; or		N/A
	b) insulated cord guard protruding >5 D (diameter)		N/A
6.10.2.2	Cord anchorage		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Protective earth conductor is the last to take the strain		N/A
	a) cord is not clamped by direct pressure from a screw		N/A
	b) knots are not used		N/A
	c) cannot push the cord into the equipment to cause a HAZARD		N/A
	d) no failure of cord insulation in anchorage with metal parts		N/A
	e) not to be loosened without a tool		N/A
	f) cord replacement does not cause a HAZARD and method of strain relief is clear		N/A
	Push-pull and or torque test	(see Form A.19)	N/A
6.10.3	Plugs and connectors		N/A
	MAINS supply plugs, connectors etc., conform with relevant specifications		N/A
	If equipment supplied at voltages below 6.3.2.a) or from a sole source:		—
	Plugs of supply cords do not fit MAINS sockets above rated SUPPLY voltage		N/A
	MAINS type plugs used only for connection to MAINS supply		N/A
	Plug pins which receive a charge from an internal capacitor	(see Form A.5)	N/A
	Accessory MAINS socket outlets:		—
	a) marking if accepts a standard MAINS supply plug (see 5.1.3e)		N/A
	b) input has a protective earth conductor if outlet has EARTH TERMINAL CONTACT		N/A
<b>6.11</b>	<b>Disconnection from supply source</b>		N/A
6.11.1	Disconnects all current-carrying conductors		N/A
6.11.2	Exceptions		N/A
6.11.3	Requirements according to type of equipment		N/A
6.11.3.1	PERMANENTLY CONNECTED EQUIPMENT and multi-phase equipment		N/A
	Employs switch or circuit-breaker		N/A
	If switch or circuit-breaker is not part of the equipment, documentation requires:		—
	a) switch or circuit-breaker to be included in building installation		N/A
	b) suitable location easily reached		N/A
	c) marking as disconnecting for the equipment		N/A
6.11.3.2	Single-phase cord-connected equipment		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Equipment is provided with one of the following:		—
	a) switch or circuit-breaker		N/A
	b) appliance coupler (disconnectable without tool)		N/A
	c) separable plug (without locking device)		N/A
6.11.4	Disconnecting devices		N/A
6.11.4.1	General		N/A
	Disconnecting device part of equipment		N/A
	Electrically close to the SUPPLY		N/A
	Power-consuming components not electrically located between the supply source and the disconnecting device		N/A
	Except electromagnetic interference suppression circuits permitted to be located on the supply side of the disconnecting device		N/A
6.11.4.2	Switches and circuit-breakers		N/A
	When used as disconnection device:		—
	Circuit breaker meets the relevant requirements IEC 60947-2 and is suitable for the application		N/A
	Switch meets the relevant requirements IEC 60947-3 and is suitable for the application		N/A
	Marked to indicate function .....		—
	Not incorporated in MAINS cord		N/A
	Does not interrupt PROTECTIVE EARTH CONDUCTOR		N/A
6.11.4.3	Appliance couplers and plugs		N/A
	Where an appliance coupler or separable plug is used as the disconnecting device (see 6.11.3.2):		—
	Readily identifiable and easily reached by the operator		N/A
	Single-phase portable equipment cord length not more than 3 m		N/A
	PROTECTIVE EARTH CONDUCTOR connected first and disconnected last		N/A

<b>7</b>	<b>PROTECTION AGAINST MECHANICAL HAZARDS</b>		<b>P</b>
<b>7.1</b>	<b>General</b>		<b>P</b>
	Equipment does not cause a mechanical HAZARD in NORMAL nor in SINGLE FAULT CONDITION		<b>P</b>
	Conformity is checked by 7.2 to 7.7		<b>P</b>
<b>7.2</b>	<b>Sharp edges</b>		<b>P</b>
	Easily-touched parts are smooth and rounded		<b>P</b>
	Do not cause injury during NORMAL USE and		<b>P</b>

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Do not cause injury during SINGLE FAULT CONDITION		P
<b>7.3</b>	<b>Moving parts</b>		N/A
7.3.1	General		N/A
	HAZARDS from moving parts limited to a tolerable level with the conditions specified in 7.3.2 and 7.3.5		N/A
	RISK assessment in accordance with 7.3.3 carried out		N/A
7.3.2	Exceptions		N/A
	Access to HAZARDOUS moving parts permitted under following circumstances:		—
	a) obviously intended to operate on parts or materials external of the equipment		N/A
	inadvertent touching of moving parts minimized by equipment design (e .g. guards or handles)		N/A
	b) If OPERATOR access is unavoidable outside NORMAL USE following precautions have been taken:		—
	1) access requires TOOL		N/A
	2) statement about training in the instructions		N/A
	3) warning markings on covers prohibiting access by untrained OPERATORS		N/A
	or symbol 14 with full details in documentation		N/A
7.3.3	RISK assessment for mechanical HAZARDS to body parts		N/A
	RISK is reduced to a tolerable level by protective measures as specified in Table 12		N/A
	Minimum protective measures:		—
	A. Low level measures		N/A
	B. Moderate measures		N/A
	C. Stringent measures		N/A
7.3.4	Limitation of force and pressure	(see Form A.20)	N/A
	Following levels are met in NORMAL and SINGLE FAULT CONDITION:		—
	Continuous contact pressure below 50 N / cm <sup>2</sup> with force below 150 N		N/A
	Temporary force below 250 N for an area at least of 3 cm <sup>2</sup> for a maximum duration of 0,75 s		N/A
7.3.5	Gap limitations between moving parts	(see Form A.20)	N/A
7.3.5.1	Access normally allowed		—
	If levels of 7.3.4 exceeded and a body part may be inserted minimum gap as specified in Table 13 assured in NORMAL and in SINGLE FAULT CONDITION		N/A
7.3.5.2	Access normally prevented		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Maximum gap as specified in Table 14 assured in NORMAL and in SINGLE FAULT CONDITION		N/A
<b>7.4</b>	<b>Stability</b>		N/A
	Equipment not secured to building structure is physical stable		N/A
	Stability maintained after opening of drawers etc. by automatic means, or		N/A
	warning marking requires the application of means		N/A
	Compliance checked by following tests as applicable:	(see Form A.20A)	—
	a) 10° tilt test for other than handheld equipment		N/A
	b) multi-directional force test for equipment exceeds height of 1 m and mass of 25 kg		N/A
	c) downward force test for floor-standing equipment		N/A
	d) overload test with 4 times maximum load for castor or support foot that supports greatest load, or		N/A
	e) castor or support foot that supports greatest load removed from equipment		N/A
<b>7.5</b>	<b>Provisions for lifting and carrying</b>		N/A
7.5.1	General		N/A
	Equipment more than 18 kg..... :		N/A
	Has means for lifting or carrying; or		N/A
	Directions are given in documentation		N/A
7.5.2	Handles and grips		N/A
	Handles or grips withstand four times weight		N/A
7.5.3	Lifting devices and supporting parts		N/A
	RATED for maximum load; or		N/A
	Tested with four times maximum static load		N/A
<b>7.6</b>	<b>Wall mounting</b>		N/A
	Mounting brackets withstand four times weight	(see Form A.20B)	N/A
	One fastener removed and test repeated with two times weight	(see Form A.20B)	N/A
<b>7.7</b>	<b>Expelled parts</b>		N/A
	Equipment contains or limits the energy		N/A
	Protection not removable without the aid of a tool		N/A

<b>8</b>	<b>RESISTANCE TO MECHANICAL STRESSES</b>		P
<b>8.1</b>	<b>General</b>		P
	Equipment does not cause a HAZARD when subjected to mechanical stresses in NORMAL USE		P
	Normal protection level is 5 J		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Levels below 5 J but not less than 1 J are acceptable if all of the following criteria are met:		—
	a) Lower level justified by RISK assessment of manufacturer		N/A
	b) Equipment installed in its intended application is not easily touched		N/A
	c) Only occasional access during NORMAL USE		N/A
	d) IK code in accordance to IEC 62262 marked or symbol 14 used with full information in the documentation		N/A
	for non-metallic ENCLOSURES rated below 2 °C ambient temperature value chosen for minimum RATED temperature		N/A
	impact energies between IK values, the IK code marked for nearest lower value		N/A
	Conformity is checked by performing following tests:	(see Form A.16)	—
	1) Static test of 8.2.1		P
	2) Impact test of 8.2.2 with 5 J except for HAND-HELD EQUIPMENT		N/A
	if specified impact energy is not 5 J alternate method of IEC 62262 used		N/A
	3) Drop test of 8.3.1 or 8.3.2 except for FIXED EQUIPMENT and equipment with mass over 100 kg		P
	Equipment RATED with an impact rating of IK 08 that obviously meets the criteria		N/A
	After the tests inspection with following results:		—
	– HAZARDOUS LIVE parts above the limits of 6.3.2 not ACCESSIBLE		N/A
	– insulation pass the voltage tests of 6.8	(see Form A.30)	N/A
	i) No leaks of corrosive and harmful substances		P
	ii) ENCLOSURE shows no cracks resulting in a HAZARD		P
	iii) CLEARANCES not less than their permitted values		N/A
	iv) Insulation of internal wiring remains undamaged		N/A
	v) PROTECTIVE BARRIERS not damaged or loosened		N/A
	vi) No moving parts exposed, except permitted by 7.3		N/A
	vii) No damage which could cause spread of fire		P
<b>8.2</b>	<b>ENCLOSURE rigidity test</b>		P
8.2.1	Static test	(see Form A.21A)	P
	– 30 N with 12 mm rod applied to each part of ENCLOSURE		P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– in case of doubt test conducted at maximum RATED ambient temperature		P
8.2.2	Impact test	(see Form A.21A)	N/A
	Impact applied to any part of ENCLOSURE causing a HAZARD if damaged		N/A
	Impact energy level and corresponding IK code.....:		—
	Non-metallic ENCLOSURES cooled to minimum RATED ambient temperature if below 2 °C		N/A
<b>8.3</b>	<b>Drop test</b>	(see Form A.21B)	P
8.3.1	Other than HAND-HELD and DIRECT-PLUG-IN EQUIPMENT		N/A
	Tests conducted with a drop height or angle of .....		—
8.3.2	HAND-HELD and DIRECT-PLUG-IN EQUIPMENT		P
	Non-metallic ENCLOSURES cooled to minimum RATED ambient temperature if below 2 °C		P
	Drop test conducted with an height of 1 m		P

<b>9</b>	<b>PROTECTION AGAINST THE SPREAD OF FIRE</b>		P
<b>9.1</b>	<b>General</b>		P
	No spread of fire in NORMAL and SINGLE FAULT CONDITION		P
	MAINS supplied equipment meets requirements of 9.6 additionally		N/A
	Conformity is checked by minimum one or a combination of the following (see Figure 11):	(see Form A.22)	—
	a) SINGLE FAULT test of 4.4; or	(see Form A.1)	P
	b) Application of 9.2 (eliminating or reducing the sources of ignition); or		N/A
	c) Application of 9.3 (containment of fire within the equipment)		P
<b>9.2</b>	<b>Eliminating or reducing the sources of ignition within the equipment</b>		N/A
	a) 1) Limited-energy circuit (see 9.4); or		N/A
	2) BASIC INSULATION provided for parts of different potential; or	(see Forms A.14 and A.18)	N/A
	Bridging the insulation does not cause ignition	(see Form A.1)	N/A
	b) Surface temperature of liquids and parts (see 9.5)		N/A
	c) No ignition in circuits designed to produce heat	(see Form A.1)	N/A
<b>9.3</b>	<b>Containment of the fire within the equipment, should it occur</b>		P
9.3.1	General		P



IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Spread of fire outside equipment reduced to a tolerable level if:		—
	a) Energizing of the equipment is controlled by an OPERATOR held switch		N/A
	b) ENCLOSURE is conform with constructional requirements of 9.3.2; and		P
	Requirements of 9.5 are met		P
9.3.2	Constructional requirements		P
	a) Connectors and insulating material have flammability classification V-2 or better	(see TABLE 1.A or Form A.23)	N/A
	b) Insulated wires and cables are flame retardant (VW-1 or equivalent)	(see TABLE 1.A or Form A.23)	N/A
	c) ENCLOSURE meets following requirements:	(see Form A.22)	—
	1) Bottom and sides in arc of 5 ° (see Figure 13) to non-limited circuits (9.4) meets:		—
	i) no openings; or		P
	ii) perforated as specified in Table 16; or		N/A
	iii) metal screen with a mesh; or		N/A
	iv) baffles as specified in Figure 12		N/A
	2) Material of ENCLOSURE and any baffle or flame barrier is made of:		—
	Metal (except magnesium); or		N/A
	Non-metallic materials have flammability classification V-1 or better	(see TABLE 1.A or Form A.22)	P
	3) ENCLOSURE and any baffle or flame barrier have adequate rigidity		N/A
<b>9.4</b>	<b>Limited-energy circuit</b>	(see Form A.24)	N/A
	a) Potential not more than 30 r.m.s. and 42,4 V peak, or 60 V d.c.		N/A
	b) Current limited by one of following means:		—
	1) Inherently or by impedance (see Table 17); or		N/A
	2) Overcurrent protective device (see Table 18); or		N/A
	3) A regulating network limits also in SINGLE FAULT CONDITION (see Table 17)		N/A
	c) Is separated by at least BASIC INSULATION		N/A
	Fuse or a nonadjustable electromechanical device is used		N/A
<b>9.5</b>	<b>Requirements for equipment containing or using flammable liquids</b>		N/A
	Flammable liquids contained in or specified for use with equipment do not cause spread of fire	(see Form A.25)	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	RISK is reduced to a tolerable level:		—
	a) The temperature of surface or parts in contact with flammable liquids is 25 °C below fire point		N/A
	b) The quantity of liquid is limited		N/A
	c) Flames are contained within the equipment		N/A
	Detailed instructions for RISK-reduction provided		N/A
<b>9.6</b>	<b>Overcurrent protection</b>		N/A
9.6.1	General		N/A
	MAINS supplied equipment protected		N/A
	BASIC INSULATION between MAINS parts of opposite polarity provided	(see Forms A.14 and A.15)	N/A
	Overcurrent protection devices not fitted in the protective conductor		N/A
	Fuses or single-pole circuit-breakers not fitted in neutral (multi-phase equipment)		N/A
9.6.2	PERMANENTLY CONNECTED EQUIPMENT		N/A
	Overcurrent protection device:		—
	Fitted within the equipment; or		N/A
	Specified in manufacturer's instructions		N/A
9.6.3	Other equipment		N/A
	Protection within the equipment		N/A

<b>10</b>	<b>EQUIPMENT TEMPERATURE LIMITS AND RESISTANCE TO HEAT</b>		P
<b>10.1</b>	<b>Surface temperature limits for protection against burns</b>		P
	Easily touched surfaces within the limits in NORMAL and in SINGLE FAULT CONDITION:	(see Form A.26A)	—
	– at an specified ambient temperature of 40 °C		N/A
	– for equipment rated above 40 °C ambient temperature limits not exceeded raised by the difference to 40 °C		P
	Heated surfaces necessary for functional reasons exceeding specified values:		—
	– Are recognizable as such by appearance or function; or		N/A
	– Are marked with symbol 13		N/A
	– Guards are not removable without tool		N/A
<b>10.2</b>	<b>Temperatures of windings</b>		N/A
	Limits not exceeded in:	(see Form A.26B)	—
	NORMAL CONDITION		N/A
	SINGLE FAULT CONDITION		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
<b>10.3</b>	<b>Other temperature measurements</b>		P
	Following measurements conducted if applicable:	(see Form A.26A)	—
	a) Value of 60 °C of field-wiring terminal box not exceeded		N/A
	b) Surface of flammable liquids and parts in contact with this liquids		N/A
	c) Surface of non-metallic ENCLOSURES		P
	d) Parts made of insulating material supporting parts connected to MAINS supply		N/A
	e) Terminals carrying a current more than 0,5 A		N/A
<b>10.4</b>	<b>Conduct of temperature tests</b>		P
10.4.1	General		P
	Tests conducted under reference test conditions and manufacturer's instructions	(see Form A.26A)	P
	Tests alternatively conducted at the least favourable ambient temperature within the RATED ambient temperature .....		—
10.4.2	Temperature measurement of heating equipment		N/A
	Tests conducted in test corner	(see Form A.26A)	N/A
10.4.3	Equipment intended for installation in a cabinet or wall		N/A
	Equipment built in as specified in installation instructions	(see Form A.26A)	N/A
<b>10.5</b>	<b>Resistance to heat</b>		P
10.5.1	Integrity of CLEARANCE and CREEPAGE DISTANCES	(see Form A.16)	N/A
10.5.2	Non-metallic ENCLOSURES	(see Form A.27)	P
	Within 10 min after treatment:	Intact	—
	Equipment subjected to suitable stresses of 8.2 and 8.3 complying with criteria of 8.1		P
10.5.3	Insulating material		N/A
	a) Parts supporting parts connected to MAINS supply		N/A
	b) TERMINALS carrying a current more than 0,5 A		N/A
	Examination of material data; or		N/A
	in case of doubt:		N/A
	1) Ball pressure test; or	(see Form A.28)	N/A
	2) Vicat softening test of ISO 306	(see Form A.29)	N/A
<b>11</b>	<b>PROTECTION AGAINST HAZARDS FROM FLUIDS AND SOLID FOREIGN OBJECTS</b>		P
<b>11.1</b>	<b>General</b>		P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Protection to OPERATORS and surrounding area provided by EQUIPMENT		P
	All fluids specified by manufacturer considered		P
11.2	<b>Cleaning</b>	(see Form A.30)	P
11.3	<b>Spillage</b>	(see Form A.30)	N/A
11.4	<b>Overflow</b>	(see Form A.30)	N/A
11.5	<b>Battery electrolyte</b>		N/A
	Battery electrolyte leakage presents no HAZARD		N/A
11.6	<b>Equipment RATED with a degree of ingress protection (IP code)</b>	(see Form A.30)	N/A
11.6.1	General		N/A
	Equipment marked with IP code .....		—
	Conditions specified in the documentation		N/A
11.6.2	Conditions for testing		N/A
	Equipment in clean and new condition, all parts in place and mounted as specified by manufacturer		N/A
	Complete equipment tested, or		N/A
	representative parts tested		N/A
	HAND-HELD EQUIPMENT and PORTABLE EQUIPMENT placed in least favourable position of NORMAL use		N/A
	Other equipment positioned or installed as specified		N/A
	TERMINALS provided with protective cap or cover, are installed as specified by manufacturer		N/A
	The equipment is operating (energized) during the treatment except:		—
	a) If manufacturer specifies degrees of protection for non-operating (de-energized) equipment, or		N/A
	b) Equipment is operating or non-operating during the treatment with does not affect the test results		N/A
11.6.3	Protection against solid foreign objects (including dust)		N/A
	Applicable test of IEC 60529 for protection against solid foreign objects conducted		N/A
	Additionally inspection of equipment resulted:		—
	a) No deposit on insulation parts that could lead to a HAZARD		N/A
	b) No created accumulations that have the potential to cause spread of fire		N/A
11.6.4	Protection against water		N/A
	Applicable test of IEC 60529 for protection against water conducted		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	If any water has entered, safety is not impaired, inspection of equipment resulted:		—
	a) No deposit on insulation parts that could lead to a HAZARD		N/A
	b) Water has not reached hazardous live parts or windings which are not designed to operate when wet		N/A
	c) No accumulations near the end of cable nor enter the cable where it could cause a HAZARD		N/A
	d) No accumulations where it could lead to a HAZARD taking in consideration movement of the equipment		N/A
<b>11.7</b>	<b>Fluid pressure and leakage</b>		N/A
11.7.1	Maximum pressure .....	(see Form A.31)	—
	Maximum pressure of any part does not exceed P <sub>RATED</sub>		N/A
11.7.2	Leakage and rupture at high pressure		N/A
	Fluid-containing parts checked by inspection or if a HAZARD could arise subjected to hydraulic test, if:	(see Form A.31)	—
	a) product of pressure and volume > 200 kPa·l; and		N/A
	b) pressure > 50 kPa		N/A
	Safety evidence established by calculation in acc. to national authorities (e.g. Pressure Equipment Directive 2014/68/EU)		N/A
	Parts of refrigerating systems meets pressure-related requirements of EN 378-2 or IEC 60335-2-89 as applicable		N/A
11.7.3	Leakage from low-pressure parts	(see Form A.32)	N/A
11.7.4	Overpressure safety device		N/A
	Does not operate in NORMAL USE		N/A
	a) Connected as close as possible to parts intended to be protected		N/A
	b) Easy access for inspection, maintenance and repair		N/A
	c) Adjustment only with TOOL		N/A
	d) No discharge towards person		N/A
	e) No HAZARD from deposit of discharged material		N/A
	f) Adequate discharge capacity		N/A
	No shut-off valve between overpressure safety device and protected parts		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
<b>12</b>	<b>PROTECTION AGAINST RADIATION, INCLUDING LASER SOURCES, AND AGAINST SONIC AND ULTRASONIC PRESSURE</b>		P
<b>12.1</b>	<b>General</b>		P
	Equipment provides protection		P
<b>12.2</b>	<b>Equipment producing ionizing radiation</b>		N/A
12.2.1	Ionizing radiation	(see Form A.33)	N/A
12.2.1.1	General		N/A
	Equipment meets the following requirements:		—
	a) if intended to emit radiation meets requirements of 12.2.1.2; or		N/A
	tested, classified and marked in accordance to IEC 62598		N/A
	b) if only emits stray radiation meets requirements of 12.2.1.3		N/A
12.2.1.2	Equipment intended to emit radiation		—
	Effective dose rate of radiation measured..... :		—
	If dose rate exceeds 5 µSv/h marked with the following:		—
	a) symbol 17 (ISO 361)		
	b) abbreviations of the radionuclides..... :		—
	c) with maximum dose at 1 m; or ..... :		—
	with dose rate value between 1 µSv/h and 5 µSv/h in m..... :		—
12.2.1.3	Equipment not intended to emit radiation	(see Form A.34)	—
	Limit for unintended stray radiation of 1 µSv/h at any easily reached point kept .....		N/A
12.2.2	Accelerated electrons		N/A
	Compartments opened only by the use of a TOOL		N/A
<b>12.3</b>	<b>Optical radiation</b>		P
	No unintentional HAZARDOUS escape of optical radiation as ultraviolet, visible or infrared radiation, including light emitting diodes:		—
	– Checked by inspection; and		P
	– Radiation sources assessed in acc. to the requirements of IEC 62471, except for sources considered to be safe (Table 22) or conditionally safe (Table 23).	Indicator LEDs used.	P
	– Lamp and lamp systems assessed to Risk Groups 1, 2, or 3 of IEC 62471 are labelled in acc. to IEC 62471-2		N/A
	– If labelling impractical, lamp or lamp systems marked with symbol 14		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Protective measures, restrictions on use, and operating instructions that may be necessary are provided, including the applicable conditions of use of Table 23.		N/A
<b>12.4</b>	<b>Microwave radiation</b>		N/A
	Power density does not exceed 10 W/m <sup>2</sup> .....		N/A
<b>12.5</b>	<b>Sonic and ultrasonic pressure</b>		N/A
12.5.1	Sound level	(see Form A.35)	N/A
	No HAZARDOUS sound emission		N/A
	Maximum sound pressure level measured and calculated for maximum sound power level as specified in ISO 3746 or ISO 9614-1		N/A
	Instruction describes measures for protection		N/A
12.5.2	Ultrasonic pressure	(see Form A.36)	N/A
	Equipment not intended to emit ultrasound does not exceed limit of 110 dB between 20 kHz and 100 kHz		N/A
	Equipment intended to emit ultrasound:		N/A
	Outside useful beam does not exceed limit of 110 dB between 20 kHz and 100 kHz		N/A
	If inside useful beam above values exceeded:		—
	Marked with Symbol 14 of Table 1		N/A
	and following information in the documentation:		—
	a) dimensions of useful beam		N/A
	b) area where ultrasonic pressure exceed 110 dB		N/A
	c) maximum sound pressure inside beam area		N/A
<b>12.6</b>	<b>Laser sources</b>		P
	Equipment meets requirements of IEC 60825-1	Laser class 2 product and evaluated as per IEC/EN 60825-1 separately.	P

<b>13</b>	<b>PROTECTION AGAINST LIBERATED GASES AND SUBSTANCES, EXPLOSION AND IMPLOSION</b>		P
<b>13.1</b>	<b>Poisonous and injurious gases and substances</b>		N/A
	No hazardous substances liberated in NORMAL CONDITION and in SINGLE FAULT CONDITION		N/A
	If potentially-hazardous substances are liberated:		—
	Operator is not directly exposed to a quantity of the substance that could cause harm		N/A
	Requirements to discharge of hazardous substances during NORMAL operation in accordance to manufacturer's instructions not considered as liberation		N/A
	Attached data/test reports demonstrate conformity		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
<b>13.2</b>	<b>Explosion and implosion</b>		N/A
13.2.1	Components		N/A
	Components liable to explode:		—
	Pressure release device provided; or		N/A
	Apparatus incorporates operator protection (see also 7.7)		N/A
	Pressure release device:		—
	Discharge without danger		N/A
	Cannot be obstructed		N/A
13.2.2	Batteries and battery charging	(see Form A.37)	P
	If explosion or fire HAZARD could occur:		—
	Protection incorporated in the equipment; or		P
	Instructions specify batteries with built-in protection		P
	In case of wrong type of battery used:		—
	No HAZARD; or		N/A
	Warning by marking and within instructions		P
	Equipment with means to charge rechargeable batteries:		—
	Warning against the charging of non-rechargeable batteries; and		N/A
	Type of rechargeable battery indicated; or		P
	Symbol 14 used		N/A
	Battery compartment design		N/A
	Single component failure		P
	Polarity reversal test		P
13.2.3	Implosion of cathode ray tubes		N/A
	If maximum face dimensions > 160 mm.....:		—
	Intrinsically protected and correctly mounted; or		N/A
	ENCLOSURE provides protection:		N/A
	If non-intrinsically protected:		—
	Screen not removable without TOOL		N/A
	If glass screen, not in contact with surface of tube		N/A

<b>14</b>	<b>COMPONENTS AND SUBASSEMBLIES</b>		P
<b>14.1</b>	<b>General</b>		P
	Where safety is involved, components and subassemblies meet relevant requirements	(see TABLE 1.A)	P
<b>14.2</b>	<b>Motors</b>		N/A
14.2.1	Motor temperatures		N/A



IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Does not present a HAZARD when stopped or prevented from starting; or	(see Forms A.1 and A.26B)	N/A
	Protected by over-temperature or thermal protection device conform with 14.3		N/A
14.2.2	Series excitation motors		N/A
	Connected direct to device, if overspeeding causes a HAZARD		N/A
<b>14.3</b>	<b>Overtemperature protection devices</b>		N/A
	Devices operating in a SINGLE FAULT CONDITION	(see Form A.38)	N/A
	a) Reliable function is ensured		N/A
	b) RATED to interrupt maximum current and voltage		N/A
	c) Does not operate in NORMAL USE		N/A
	If self-resetting device used to prevent a HAZARD, protected part requires intervention before restarting		N/A
<b>14.4</b>	<b>Fuse holders</b>		N/A
	No access to HAZARDOUS LIVE parts		N/A
<b>14.5</b>	<b>MAINS voltage selecting devices</b>		N/A
	Accidental change not possible		N/A
<b>14.6</b>	<b>MAINS transformers tested outside equipment</b>	(see Forms A.39 and A.40)	N/A
<b>14.7</b>	<b>Printed wiring boards</b>		P
	Data shows conformity with V-1 of IEC 60695-11-10 or better; or		P
	Test shows conformity with V-1 of IEC 60695-11-10 or better	(see Form A.23)	N/A
	Not applicable for printed wiring boards with limited-energy circuits (9.4)		N/A
<b>14.8</b>	<b>Circuits used to limit TRANSIENT OVERVOLTAGES</b>		N/A
	Test conducted between each pair of MAINS SUPPLY TERMINALS	(see Form A.41)	N/A
	No ignition or overheating of other materials :		—
	– no ignition		N/A
	– no heat to other parts above the self-ignition points		N/A
	Safely suppressing and properly functional after applied tests		N/A

<b>15</b>	<b>PROTECTION BY INTERLOCKS</b>		N/A
<b>15.1</b>	<b>General</b>		N/A
	Interlocks are designed to remove a HAZARD before OPERATOR exposed		N/A
<b>15.2</b>	<b>Prevention of reactivation</b>		N/A
<b>15.3</b>	<b>Reliability</b>		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Single fault unlikely to occur; or		N/A
	Cannot cause a HAZARD		N/A

<b>16</b>	<b>HAZARDS RESULTING FROM APPLICATION</b>		P
<b>16.1</b>	<b>REASONABLY FORESEEABLE MISUSE</b>		P
	No HAZARDS arising from settings not intended and not described in the instructions		P
	Other cases of REASONABLY FORESEEABLE MISUSE addressed by RISK assessment		N/A
<b>16.2</b>	<b>Ergonomic aspects</b>		N/A
	Factors giving rise to a HAZARD the RISK assessment is reflecting those aspects:		—
	a) limitation of body dimensions		N/A
	b) displays and indicators		N/A
	c) accessibility and conventions of controls		N/A
	d) arrangement of TERMINALS		N/A

<b>17</b>	<b>RISK ASSESSMENT</b>		N/A
	RISK assessment conducted, if HAZARD might arise and not covered by Clauses 6 to 16		N/A
	TOLERABLE RISK achieved by iterative documented process covering the following:		—
	a) RISK analysis		N/A
	Identifies HAZARDS and estimates RISK		N/A
	b) RISK evaluation		N/A
	Plan to judge acceptability of resulting RISK level based on the estimated severity and likelihood of a RISK		N/A
	c) RISK reduction		N/A
	Initial RISK reduced by counter measures;		N/A
	Repeated RISK evaluation without new RISKS introduced		N/A
	RISKS remaining after RISK assessment addressed in instructions to RESPONSIBLE BODY:		—
	Information contained how to mitigate these RISKS		N/A
	Following principles in methods of RISK reduction applied by manufacturer in given order:		—
	1) RISKS eliminated or reduced as far as possible		N/A
	2) Protective measures taken for RISKS that cannot be eliminated		N/A
	3) User information about residual RISK due to any defect of the protective measures		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Indication of particular training is required		N/A
	Specification of the need for personal protective equipment		N/A
	Conformity checked by evaluation of the RISK assessment documentation		N/A

<b>ANNEX F</b>	<b>ROUTINE TESTS</b>		N/A
	Manufacturer ´s declaration		N/A

<b>ANNEX H</b>	<b>QUALIFICATION OF CONFORMAL COATINGS FOR PROTECTION AGAINST POLLUTION</b>		N/A
<b>H.1</b>	<b>General</b>		N/A
	Conformal coatings meet the requirements of Clause H.2 and H.3.		N/A
<b>H.2</b>	<b>Technical properties</b>		N/A
	Technical properties of conformal coatings are suitable for the intended application. In particular:		—
	a) Manufacturer indicate that it is a coating for PWBs;		N/A
	b) RATED operating temperature include the temperature range of the indicated application;		N/A
	c) CTI, insulation resistance and dielectric strength are suitable for the intended application;		N/A
	d) Coating have adequate UV resistance, if it is exposed to sunlight;		N/A
	e) Flammability RATING of the coating is at least the required flammability RATING of the applied PWB.		N/A
<b>H.3</b>	<b>Qualification of coatings</b>	(see Form A.42)	N/A
	Coating complies with the conformity requirements.		N/A

<b>ANNEX K</b>	<b>INSULATION REQUIREMENTS NOT COVERED BY CLAUSE 6.7</b>	(see Forms A.15 and A.18)	N/A
			N/A

IEC 61010-1					
Clause	Requirement — Test			Result — Remark	Verdict
<b>4.4</b>	<b>TABLE: Testing in SINGLE FAULT CONDITION – Results</b>			<b>Form A.1</b>	<b>P</b>
Test subclause	Fault No.	Fault description	Td 4.4.3 (NOTE)	How was test terminated Comments	Meets 4.4.4
4.4.2.8	1	Micro USB SC	00:10:00	Powered by lithium battery pack, unit was operating normally, no damage, no hazards.	P
4.4.2.8	2	Lithium battery pack output SC	00:10:00	Lithium battery pack shut down, no damage, no hazards.	P
4.4.1	3	Lithium battery pack overcharge UP1 Pin 1,24 to Pin 13,14 SC	07:00:00	Input: 5 V d.c., 2,62 A, 2,39 A for battery pack charge circuit, No damage, no hazards. See appended table 10.3 for details	P
4.4.1	4	Lithium battery pack overcharge Q2 Pin 1,3-4,6 SC	07:00:00	Input: 5 V d.c., 1,01 A, 0,99 A for battery pack charge circuit, No damage, no hazards. See appended table 10.3 for details	P
4.4.1	5	Lithium battery pack rapid discharge UP1 Pin 1,24 to Pin 13,14 SC	06:50:00	Powered by lithium battery pack, 0,34 A, No damage, no hazards.	P
4.4.1	6	Lithium battery pack rapid discharge P1 SC	00:10:00	Powered by lithium battery pack, 0,25 A, No damage, no hazards.	P
NOTE Td = Test duration in hh:mm:ss Record dielectric strength test on Form A.18 and temperature tests on Forms A.26A and / or A.26B. Record in the comments column for each test whether carried out during or after SINGLE FAULT CONDITION.					
Supplementary information:					

IEC 61010-1						
Clause	Requirement — Test	Result — Remark	Verdict			
<b>5.1.3c)</b>	<b>TABLE: MAINS supply</b>	<b>Form A.2</b>	<b>P</b>			
	Marked rating..... :	5 V	—			
	Phase..... :	-	—			
	Frequency ..... :	- Hz	—			
	Current ..... :	1,1 A	—			
	Power ..... :	5,5 W	—			
	Power ..... :	- VA	—			
Test No.	Voltage [V]	Frequency [Hz]	Current [A]	Power		Comments
				[W]	[VA]	
1	5	-	1,01	5,05	-	0,99A for battery charge current. Exhausted battery charged through USB port and EUT was working under max. normal condition
2	-	-	0,25	-	-	Powered by full battery and EUT was working under max. normal condition
-						
-						
-						
-						
-						
-						
-						
-						
-						
-						
-						
-						
-						
NOTE – Measurements are only required for marked ratings. Initial inrush currents are not regarded.						
Supplementary information:						

IEC 61010-1					
Clause	Requirement — Test			Result — Remark	Verdict
<b>5.3</b>	<b>TABLE: Durability of markings</b>			<b>Form A.3</b>	<b>P</b>
Marking method (see NOTE)			Agent		
1) Adhesive label			A Water		
2) Ink printed			B Pure ethanol		
3) Laser marked			C (specify agent)		
4) Film-coated (plastic foil control panel)			D (specify agent)		
5) Imprinted on plastic (moulded in)			E (specify agent)		
NOTE – Where applicable include print method, label material, ink or paint type, fixing method, adhesive and surface to which marking is fixed.					
Marking location			Marking method (see above)		
Identification (5.1.2)			1), 2)		
MAINS supply (5.1.3)			1), 2)		
Fuses (5.1.4)			N/A		
Terminals and operating devices (5.1.5.2)			N/A		
Switches and circuit breakers (5.1.6)			N/A		
Double/reinforced equipment (5.1.7)			N/A		
Field wiring Terminal boxes (5.1.8)			N/A		
Warning marking (5.2)			1), 2)		
Battery charging (13.2.2)			N/A		
Method	Test agent	Remains legible	Label loose	Curled edges	Comments
		Verdict	Verdict	Verdict	
1)	A	Yes	No	No	
2)	A	Yes	No	No	
1)	B	Yes	No	No	
2)	B	Yes	No	No	
Supplementary information:					



IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>6</b>	<b>TABLE: Values in NORMAL CONDITION</b>										<b>Form A.5</b>	<b>P</b>	
6.1.2	Exceptions							11.2 Cleaning and decontamination			—		
6.3.1	Values in NORMAL CONDITION (see NOTE 1)							11.3 Spillage			—		
6.6.2	Terminals for external circuit							11.4 Overflow			—		
6.10.3	Plugs and connections										—		
Item (see Form A.4)	Voltage			Current				Capacitance		10 s / 5 s test (NOTE)			Comments
	V r.m.s.	V peak	V d.c.	Test circuit A1/A2/A3	mA r.m.s.	mA peak	mA d.c.	μC	mJ	V	μC	mJ	
1	-	-	5 Vdc	-	-	-	-	-	-	-	-	-	
2	-	-	5 Vdc	-	-	-	-	-	-	-	-	-	

NOTE – A 10 s test is specified in 6.1.2 a) b). A. 5 s test is specified in 6.10.3. The capacitance level versus voltage below the limits given from figure 3 of IEC 61010-1.

Supplementary information:



IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

6.3.2	TABLE: Values in SINGLE FAULT CONDITION											Form A.6	P
Item  (see Form A.4)	Subclause and fault No. (see Form A.1)	Voltage			Transient (see NOTE)		Current				Capacitance	Comments	
	V r.m.s.	V peak	V d.c.	V	s	Test circuit A1/A2/A3	mA r.m.s.	mA peak	mA d.c.	µF (see NOTE)			
1	1-6	-	-	5 Vdc	-	-	-	-	-	-	-		
2	1-6	-	-	5 Vdc	-	-	-	-	-	-	-		

NOTE – Transient voltages must be below the limits given from Figure 2 and the capacitance below the limits from figure 3 of IEC 61010-1.

Supplementary information:

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict
<b>6.5.2.2</b>	<b>TABLE: Cross-sectional area of bonding conductors</b>	<b>Form A.7</b>	N/A
Conductor location	CROSS-SECTIONAL AREA [mm <sup>2</sup> ]		Verdict
Supplementary information:			
<b>6.5.2.3</b>	<b>TABLE: Tightening torque test</b>	<b>Form A.8</b>	N/A
Conductor location	Size of screw	Tightening torque [Nm]	Verdict
Supplementary information:			

IEC 61010-1				
Clause	Requirement — Test	Result — Remark		Verdict
<b>6.5.2.4</b>	<b>TABLE: BONDING impedance of plug-connected equipment</b>			<b>Form A.9</b>
				N/A
	<b>ACCESSIBLE part under test</b>	<b>Test current</b> [A]	<b>Voltage attained after 1 min</b> [V]	<b>Calculated resistance</b> (Maximum 0,1 or 0,2 Ω) [Ω] (NOTE 1)
				Verdict
NOTE 1 – For none-detachable power cord the impedance between protective conductor plug pin of MAINS cord and each ACCESSIBLE part shall not exceed 0,2 Ohm.				
Supplementary information:				
<b>6.5.2.5</b>	<b>TABLE: BONDING impedance of PERMANENTLY CONNECTED EQUIPMENT</b>			<b>Form A.10</b>
				N/A
	<b>ACCESSIBLE part under test</b>	<b>Test current</b> [A]	<b>Voltage attained after 1 min</b> (maximum 10 V) [V]	<b>Verdict</b>
Supplementary information:				
<b>6.5.2.6</b>	<b>TABLE: Transformer PROTECTIVE BONDING screen</b>			<b>Form A.11</b>
				N/A
	<b>ACCESSIBLE part under test</b>	<b>Test current</b> (see NOTE) [A]	<b>Voltage attained after 1 min</b> (maximum 10 V) [V]	<b>Calculated resistance</b> (maximum 0,1 Ω) [Ω]
				Verdict
NOTE – Test current must be twice the value of the overcurrent protection means of the winding. Test is specified in 6.5.2.6 a) or b).				
Supplementary information:				

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>6.5.4</b>	<b>TABLE: PROTECTIVE IMPEDANCE</b>	<b>Form A.12</b>	N/A
--------------	------------------------------------	------------------	-----

A single component								
Component	Location	Measured		Calculated	Rated		Verdict	Comments
		Working voltage [V]	Current [A]	Power dissipation [W]	Working voltage [V]	Power dissipation [W]		

A combination of components		
Component	Location	Comments

NOTE – A PROTECTIVE IMPEDANCE shall not be a single electronic device that employs electron conduction in a vacuum, gas or semiconductor.

Supplementary information:

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>6.5.6</b>	<b>TABLE: Current- or voltage-limiting device</b>					<b>Form A.13</b>	N/A
Component	Location	Measured		Rated		Verdict	Comments
		Working voltage [V]	Current [A]	Working voltage [V]	Current [A]		

Supplementary information:

IEC 61010-1												
Clause	Requirement — Test	Result — Remark	Verdict									
<b>6.7</b>	<b>TABLE: Insulation requirements - Block diagram of system -</b>	<b>Form A.14</b>	<b>N/A</b>									
Pollution degree..... :						Overvoltage category.....:						
Area	Location	Insulation type (NOTE 1)	WORKING VOLTAGE			CLEARANCE (NOTE 3) [mm]	CREEPAGE DISTANCE (NOTE 3)				Test voltage (NOTE 2) [V]	Comments (NOTE 3)
			RMS [V]	Peak [V]	Freq. [kHz]		PWB [mm]	CTI	Other [mm]	CTI		
A												
B												
C												
D												
E												
F												
NOTE 1 – Type of insulation: BI = BASIC INSULATION DI = DOUBLE INSULATION PI = PROTECTIVE IMPEDANCE RI = Reinforced INSULATION SI = Supplementary INSULATION see also Form A.15 for further details			NOTE 2 - Types of voltage Peak impulse test voltage (pulse) r.m.s. d.c. peak				NOTE 3 - OVERVOLTAGE CATEGORIES or POLLUTION DEGREES which differ should be shown under "Comments"					
<b>Supplementary Information:</b> EUT was powered by building-in 3,6Vdc lithium battery pack and 5Vdc power source.no boosted hazardous circuits exist.												

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>6.7</b>	<b>TABLE: Insulation requirements - CLEARANCES and CREEPAGES</b>	<b>Form A.15</b>	N/A
6.2.2	Examination	6.5.4 Protective impedance	—
6.4.2	ENCLOSURES and protective barriers	6.5.6 Current- or voltage-limiting device	—
6.4.4	Impedance	9.6.1 BASIC INSULATION between opposite polarity	—

Area	Location (See Form A.14)	Insulation type (NOTE 1)	WORKING VOLTAGE (NOTE 2)			CLEARANCE		CREEPAGE DISTANCE		CTI	Verdict	Comments
			RMS [V]	Peak [V]	Frequency [kHz]	Required [mm]	Measured [mm]	Required [mm]	Measured [mm]			
A												
B												
C												
D												
E												
F												

NOTE 1 – refer to Form A.14 for type of insulation shown in the insulation diagram      NOTE 2 - to be used for definition of required insulation (see Form A.14)

Input supply voltage.....:		V		Hz
----------------------------	--	---	--	----

Supplementary information:  
 EUT was powered by building-in 3,6Vdc lithium battery pack and 5Vdc power source.no boosted hazardous circuits exist.

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>6.7</b>	<b>TABLE: Insulation requirements - CLEARANCES and CREEPAGES</b>		<b>Form A.16</b>	N/A
6.4.2	ENCLOSURES or PROTECTIVE BARRIERS	9.6.1	Overcurrent protection basic insulation between MAINS parts	—
8	Mechanical resistance to shock and impact	10.5.1	Integrity of CLEARANCES and CREEPAGE DISTANCES	—

Area	Location (See Form A.14)	Insulation type	Mechanical tests (NOTE)					Test at max.  RATED ambient (10.5.1)	Measured after test (if required)		Verdict	Comments
			Applied force  [N]	Rigidity (8.2)		Drop (8.3)			CLEARANCE  [mm]	CREEPAGE DISTANCE  [mm]		
				Static (8.2.1)	Impact (8.2.2)	Normal (8.3.1)	Hand-held/ Plug-in					
A												
B												
C												
D												
E												
F												

NOTE – Refer to Form A.18 for dielectric strength tests following the above tests.

Supplementary information:  
 EUT was powered by building-in 3,6Vdc lithium battery pack and 5Vdc power source.no boosted hazardous circuits exist.



IEC 61010-1							
Clause	Requirement – Test	Result — Remark	Verdict				
<b>6.7.2.2.2</b>	<b>TABLE: Reliability of potted components</b>	<b>Form A.17 (optional)</b>	N/A				
<b>14.1 b)</b>	<b>Components and subassemblies</b>		N/A				
<b>Temperature Cycling Test</b>							
Manufacturer .....							
Type.....							
Construction .....							
Potting compound .....							
CREEPAGE DISTANCES measured .....							
CLEARANCES measured .....							
Thickness through insulation.....							
Adhesive test Pass/Fail .....							
Test temperature T °C.....							
Cycles at U= AC 500 V					Leakage current (at AC 500 V) mA		
Number of cycles	Date			68 h /	1 h /	2 h /	1 h /
				125 °C	25 °C	0 °C	25 °C
1. Cycle from		to					
2. Cycle from		to					
3. Cycle from		to					
4. Cycle from		to					
5. Cycle from		to					
6. Cycle from		to					
7. Cycle from		to					
8. Cycle from		to					
9. Cycle from		to					
10. Cycle from		to					
After Cycling Test :							
Humidity conditioning					48 h		
Requirements for dielectric strength (s. insulation diagram)					Test voltage V r.m.s.		Verdict
Basic insulation _____ V r.m.s.							
Supplementary insulation _____ V r.m.s.							
Reinforced insulation _____ V r.m.s.							
NOTE - to be used for evaluation of components containing insulation through solid insulation, when the component standard require thermal cycling test. Ref Clause 14.1 and Figure 15, option b)							
Supplementary information:							





IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>7.</b>	<b>TABLE: Protection against mechanical HAZARDS</b>	<b>Form A.20</b>	N/A
7.3.4	Limitation of force and pressure		—
7.3.5	Gap limitations between moving parts		—

Part / Location	Clause 7.3.4		Clause 7.3.5.1								Clause 7.3.5.2			Verdict	Comments
	Continuous	Temporary	Minimum gaps [mm]								Maximum gaps [mm]				
	Contact pressure max. 50 N /cm <sup>2</sup> @ max. 150 N	max. 250 N / 3 cm <sup>2</sup> @ max. 0,75 s	Torso 500	Head 300	Leg 180	Foot 120	Toes 50	Arm 120	Hand 100	Finger 25	Head 120	Foot 35	Finger 4		

Supplementary information:

IEC 61010-1							
Clause	Requirement – Test				Result - Remark		Verdict
<b>7.4</b>	<b>TABLE: Stability</b>				<b>Form A.20A</b>		N/A
	Equipment height / mass .....				mm	kg	—
	Equipment (Containers) loaded.....				[yes / no]		—
	Castors at unfavourable position.....				[yes / no]		—
	Doors, drawers and movable arms closed.....				[yes / no]		—
	Doors and drawers at unfavourable position.....				[yes / no]		—
Location	Tilt angle	Applied force				Comments	Verdict
	10°	250 N	20% [N]	800 N	4 times load [N]		
Front side				—			
Left side				—			
Rear side				—			
Right side				—			
Top side	—						
Working surface	—	—	—				
Ledge	—	—	—				
Castor / support foot							
Castor / support foot removed							
Supplementary information:							
<b>7.6</b>	<b>TABLE: Wall mounting</b>				<b>Form A.20B</b>		N/A
	Equipment weight .....				kg		—
	Equipment mounted as specified by manufacturer ..				[yes / no]		—
	Equipment mounted at plasterboard (drywall) .....				[yes / no]		—
	More than one fastener used .....				[yes / no]		—
	Test maintained (after 5 s to 10 s to full load) .....				1 min		—
Location	Applied weight				Comments	Verdict	
	4 times weight [kg]		2 times weight [kg]				
Mounting brackets							
Supplementary information:							

IEC 61010-1			
Clause	Requirement – Test	Result - Remark	Verdict
<b>8.2</b>	<b>TABLE: ENCLOSURE rigidity test</b>	<b>Form A.21A</b>	<b>P</b>
8.2.1	Static test		P
	Material of enclosure .....	non-metallic	—
	Preparation for the test:		—
	Operated at ambient temperature .....	50 °C   3 h	—
	Location	Comments	Verdict
	1) Enclosure near battery	Intact	P
	2)		
	3)		
	4)		
Supplementary information:			
<b>8.2.2</b>	<b>TABLE: Impact test</b>		<b>N/A</b>
	Material of enclosure .....	Metal / non-metallic	—
	Corresponding IK-code.....		—
	Preparation for the test:		—
	Cooled to (temperature) .....	°C	—
	Location	Comments	Verdict
	1) Top		
	2) Side left / right		
	3) Bottom		
Supplementary information:			

IEC 61010-1					
Clause	Requirement – Test	Result - Remark		Verdict	
<b>8.3</b>	<b>TABLE: Drop test</b>	<b>Form A.21B</b>		<b>P</b>	
8.3.1	Other equipment			N/A	
	Location	Raised up to		Comments	—
		[mm]	30 °		
1)					
2)					
3)					
4)					
Supplementary information:					
8.3.2	HAND-HELD EQUIPMENT and DIRECT PLUG-IN EQUIPMENT			<b>P</b>	
	Material of enclosure .....	non-metallic		—	
	Preparation for the test:			—	
	Cooled to (temperature) .....	-10 °C		—	
	Location	Comments		Verdict	
1)	Side	Intact		P	
2)	Edge	Intact		P	
3)	Corner	Intact		P	
Supplementary information:					

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>9</b>	<b>TABLE: Protection against the spread of fire</b>		<b>Form A.22</b>	<b>P</b>
Item	Source of HAZARD or area of the equipment considered (circuit, component, liquid etc.)	Protection Method (9.1 a, b or c)	Protection details	Verdict
1	Battery	9.1 a,c	Fire enclosure was provided.	P
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				
-				

Supplementary information:



IEC 61010-1									
Clause	Requirement — Test	Result — Remark				Verdict			
9.3.2	<b>TABLE: Constructional requirements</b>	<b>Form A.23</b>				N/A			
14.7	Printed wiring boards					N/A			
Material tested .....									
Generic name .....									
Material manufacturer .....									
Type .....									
Colour .....									
Conditioning details .....									
				Sample					
				1	2	3	4	5	6
Thickness of specimen	mm								
Duration of flaming after first Application	s								
Duration of flaming plus glowing After second application	s								
Specimen burns to holding clamp	Yes/No								
Cotton ignited	Yes/No								
Sample result	Pass/Fail								
Supplementary information:									

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>9.4</b>	<b>TABLE: Limited-energy circuit</b>	<b>Form A.24</b>	N/A
------------	--------------------------------------	------------------	-----

Item or Location  (see Form A.22)	9.4 a)	9.4 b) Current limitation (NOTE)		9.4 c)	Decision	Comments
	Maximum potential in circuit voltage r.m.s./d.c. [V]	Maximum available current [A]	Overload protection after 120 s [A]	Circuit separation	Yes/No	

NOTE – Maximum values see Tables 17 and 18 of IEC 61010-1

Supplementary information:



IEC 61010-1					
Clause	Requirement — Test	Result — Remark			Verdict
<b>10.</b>	<b>TABLE: Temperature Measurements</b>	<b>Form A.26A</b>			<b>P</b>
10.1	Surface temperature limits – NORMAL CONDITION				P
10.2	Temperature of windings – NORMAL CONDITION				N/A
10.3	Other temperature measurements				P
Operating conditions:		Exhausted battery charged through USB port and EUT was working under max. normal condition			
Frequency..... :	- Hz	Test room ambient temperature (ta).... :	23,5 °C		
Voltage..... :	5 V	Test duration..... :	1 h 11 min		
Part / Location	$t_m$ [°C]	$t_c$ [°C]	$t_{max}$ [°C]	Verdict	Comments
LCD panel	33.2	59.7	85	P	
Press button	33.6	60.1	70	P	
Outside of plastic enclosure near camera	33.4	59.9	85	P	
Inside of plastic enclosure near camera	30.1	56.6	85	P	
Outside of plastic enclosure near battery cell	28.4	54.9	85	P	
Inside of plastic enclosure near battery cell	28.5	55.0	85	P	
Battery cell	31.7	58.2	Ref.	P	
Laser module heatsink	34.6	61.1	Ref.	P	
PCB near 1	44.1	70.6	130	P	
PCB near 2	49.6	76.1	130	P	
PCB near 3	41.7	68.2	130	P	
PCB near 4	42.8	69.3	130	P	
PCB near 5	41.8	68.3	130	P	
-					
-					
-					
-					
-					
NOTE 1 - $t_m$ = measured temperature $t_c = t_m$ corrected ( $t_m - t_a + 50\text{ °C}$ or max. RATED ambient) $t_{max}$ = maximum permitted temperature NOTE 2 - see also 14.1 with reference to component operating conditions NOTE 3 - Record values for NORMAL CONDITION and / or SINGLE FAULT CONDITION in this Form use additional form if necessary NOTE 4 - see Form A.26B for details of winding temperature measurements Supplementary information:					

IEC 61010-1					
Clause	Requirement — Test	Result — Remark			Verdict
<b>10.</b>	<b>TABLE: Temperature Measurements</b>	<b>Form A.26A</b>			<b>P</b>
10.1	Surface temperature limits – NORMAL CONDITION				P
10.2	Temperature of windings – NORMAL CONDITION				N/A
10.3	Other temperature measurements				P
Operating conditions:		Powered by full battery and EUT was working under max. normal condition			
Frequency..... :	- Hz	Test room ambient temperature (ta).... :	27,3 °C		
Voltage..... :	- V	Test duration..... :	1 h 15 min		
Part / Location	$t_m$ [°C]	$t_c$ [°C]	$t_{max}$ [°C]	Verdict	Comments
LCD panel	32,9	55,6	85	P	
Press button	32,3	55,0	70	P	
Outside of plastic enclosure near camera	35,2	57,9	85	P	
Inside of plastic enclosure near camera	31,4	54,1	85	P	
Outside of plastic enclosure near battery cell	28,6	51,3	85	P	
Inside of plastic enclosure near battery cell	28,4	51,1	85	P	
Battery cell	29,0	51,7	Ref.	P	
Laser module heatsink	35,8	58,5	Ref.	P	
PCB near 1	42,5	65,2	130	P	
PCB near 2	47,0	69,7	130	P	
PCB near 3	40,3	63,0	130	P	
PCB near 4	39,7	62,4	130	P	
PCB near 5	38,5	61,2	130	P	
-					
-					
-					
-					
-					
NOTE 1 - $t_m$ = measured temperature $t_c$ = $t_m$ corrected ( $t_m - t_a + 50$ °C or max. RATED ambient) $t_{max}$ = maximum permitted temperature NOTE 2 - see also 14.1 with reference to component operating conditions NOTE 3 - Record values for NORMAL CONDITION and / or SINGLE FAULT CONDITION in this Form use additional form if necessary NOTE 4 - see Form A.26B for details of winding temperature measurements					
Supplementary information:					

<b>10.</b>	<b>TABLE: Temperature Measurements</b>			<b>Form A.26A</b>	<b>P</b>	
10.1	Surface temperature limits – SINGLE FAULT CONDITION, SEE BELOW				<b>P</b>	
10.2	Temperature of windings – NORMAL CONDITION				<b>N/A</b>	
10.3	Other temperature measurements				<b>P</b>	
Operating conditions:		1) Lithium battery pack overcharge UP1 Pin 1,24 to Pin 13,14 SC, 2) Lithium battery pack overcharge Q2 Pin 1,3-4,6 SC, 3) Lithium battery pack rapid discharge UP1 Pin 1,24 to Pin 13,14 SC				
Frequency..... :	- Hz	Test room ambient temperature (ta).... :		1) 16,0°C 2) 15,0°C 3) 22,8°C		
Voltage..... :	1), 2) 5 V	Test duration..... :		1)7 h 00 min 2)7 00 3)7 00		
Part / Location		$t_m$ [°C]	$t_c$ [°C]	$t_{max}$ [°C]	Verdict	Comments
LCD panel		29,0	62,0	105	P	1)
Press button		28,0	64,8	105	P	1)
Outside of plastic enclosure near camera		30,8	59,5	105	P	1)
Outside of plastic enclosure near battery cell		25,5	60,4	105	P	1)
Battery cell		26,4	62,0	Ref.	P	1)
LCD panel		31,4	66,5	105		2)
Press button		31,3	66,4	105		2)
Outside of plastic enclosure near camera		32,7	67,8	105		2)
Outside of plastic enclosure near battery cell		25,6	60,7	105		2)
Battery cell		27,5	62,6	Ref.		2)
LCD panel		30,4	57,6	105		3)
Press button		29,4	56,6	105		3)
Outside of plastic enclosure near camera		32,3	59,5	105		3)
Outside of plastic enclosure near battery cell		26,9	54,1	105		3)
Battery cell		26,4	53,6	Ref.		3)
<p>NOTE 1 - <math>t_m</math> = measured temperature  <math>t_c = t_m</math> corrected (<math>t_m - t_a + 50\text{ °C}</math> or max. RATED ambient)  <math>t_{max}</math> = maximum permitted temperature</p> <p>NOTE 2 - see also 14.1 with reference to component operating conditions</p> <p>NOTE 3 - Record values for NORMAL CONDITION and / or SINGLE FAULT CONDITION in this Form use additional form if necessary</p> <p>NOTE 4 - see Form A.26B for details of winding temperature measurements</p>						
Supplementary information:						







IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict
<b>10.5.3</b>	<b>TABLE: Insulating material</b>	<b>Form A.28</b>	N/A
10.5.3 1)	Ball-pressure test		N/A
	Max. allowed impression diameter .....	2 mm	—
Part	Test temperature [°C]	Impression diameter [mm]	Verdict
Supplementary information:			
10.5.3 2)	<b>Vicat softening test (ISO 306)</b>	<b>Form A.29</b>	N/A
Part	Vicat softening temperature [°C]	Thickness of sample [mm]	Verdict
Supplementary information:			

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>8</b>	<b>TABLE: Mechanical resistance to shock and impact</b>	<b>Form A.30</b>	P
<b>11</b>	<b>Protection against HAZARDS from fluids and solid foreign objects</b>		P

Voltage tests can be carried out once after performing the tests of clause 8 and clause 11. However, if voltage tests are carried out separately after each set of tests, two forms can be used.

Location (see Form A.14)	Clause 8 tests				Clause 11 tests				Working voltage [r.m.s./d.c.]	Test voltage [r.m.s./peak/d.c.]	Verdict	Comments
	Static (8.2.1) 30 N	Impact (8.2.2)	Normal (8.3.1)	Handheld Plug-in (8.3.2)	Cleaning (11.2)	Spillage (11.3)	Overflow (11.4)	IEC 60529 (11.6)				
Enclosure	Yes	No	No	Yes	Yes	No	No	No	No	No	P	

NOTE – Use r.m.s., d.c. or peak to indicate the used test voltage.

Supplementary information:

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

<b>11.7.2</b>	<b>TABLE: Leakage and rupture at high pressure</b>					<b>Form A.31</b>	N/A
Part	Maximum permissible working pressure [MPa]	Test pressure [MPa]	Leakage Yes / No	Deformation Yes / No	Burst Yes / No	Comments	

NOTE – see also Annex G with requirements for USA and Canada.  
 Supplementary information:

<b>11.7.3</b>	<b>TABLE: Leakage from low-pressure parts</b>			<b>Form A.32</b>	N/A
Part	Test pressure [MPa]	Leakage Yes / No	Comments		

Supplementary information:


IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict
<b>12.2.1</b>	<b>TABLE: Ionizing radiation</b>	<b>Form A.33</b>	N/A
12.2.1.2	Equipment intended to emit radiation		N/A
Locations tested	Measured values [μSv/h]	Verdict	Comments
Supplementary information:			
<b>12.2.1.3</b>	<b>Equipment not intended to emit radiation</b>	<b>Form A.34</b>	N/A
	Max. allowed effective dose rate at 100 mm.....:	1 μSv/h	—
Locations tested	Measured values [μSv/h]	Verdict	Comments
Supplementary information:			

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict
<b>12.5.1</b>	<b>TABLE: Sound level</b>	<b>Form A.35</b>	<b>N/A</b>
Locations tested	Measured maximum sound pressure level dB(A)	Calculated maximum sound power level	
At operator's normal position and at bystanders' positions			
a)			
b)			
c)			
d)			
e)			
f)			
Supplementary information:			
<b>12.5.2</b>	<b>TABLE: Ultrasonic pressure</b>	<b>Form A.36</b>	<b>N/A</b>
Locations tested	Measured values		Comments
	[dB]	[kHz]	
At operator's normal position			
At 1 m from the ENCLOSURE			
a)			
b)			
c)			
d)			
e)			
NOTE – No limit is specified at present, but a limit of 110 dB above the reference pressure value of 20 µPa is under consideration for applicable frequencies between 20 kHz and 100 kHz.			
Supplementary information:			


IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

13.2.2	<b>TABLE: Batteries and battery charging</b>	<b>Form A.37</b>	P
--------	--	------------------	---

	Battery load and charging circuit diagram:		P
--	--	--	---

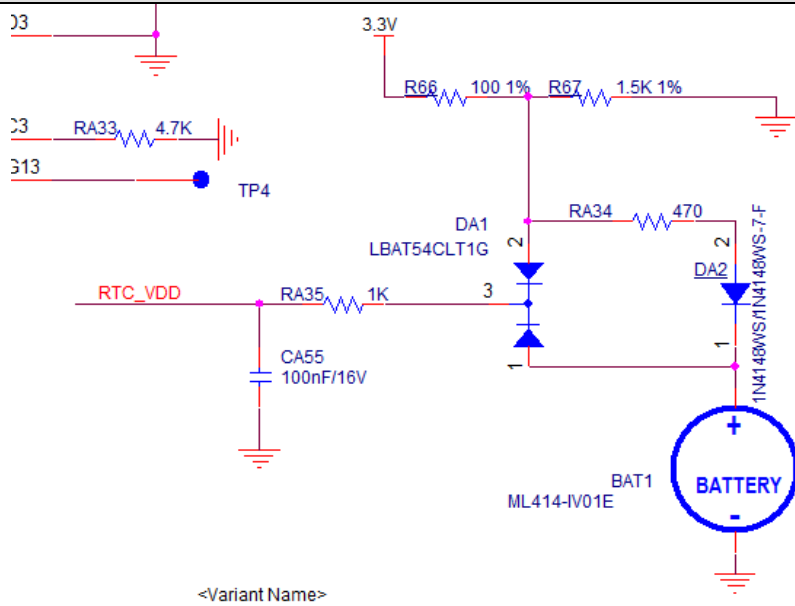

RTC protection circuits

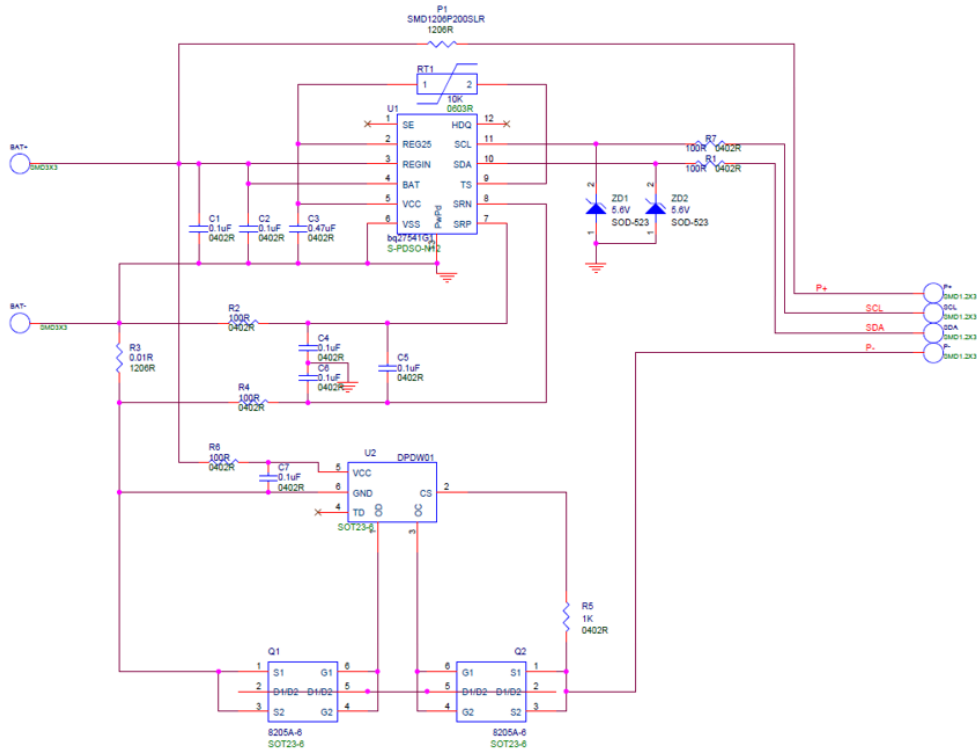

Battery pack protection circuits

	Battery type .....	See table 1.A for details	—
	Battery manufacturer/model/catalogue No. ....	See table 1.A for details	—
	Battery ratings .....	See table 1.A for details	—
	Reverse polarity instalment test		P
Single component failures		Verdict	

IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict
<b>13.2.2</b>	<b>TABLE: Batteries and battery charging</b>	<b>Form A.37</b>	<b>P</b>
	Battery load and charging circuit diagram:		<b>P</b>
Component		Open circuit	Short circuit
For RTC circuits		-	-
DA1 pin 1-2 SC (Overcharge)		-	31,25mA
CA55 (Rapid discharge)		-	1,46mA
For battery pack		-	-
Lithium battery pack overcharge UP1 Pin 1,24 to Pin 13,14 SC		-	2,39A
Lithium battery pack overcharge Q2 Pin 1,3-4,6 SC		-	0,99A
Lithium battery pack rapid discharge UP1 Pin 1,24 to Pin 13,14 SC		-	0,34A
Lithium battery pack rapid discharge P1 SC		-	0,25A
Supplementary information:			





IEC 61010-1				
Clause	Requirement — Test	Result — Remark		Verdict
<b>4.4.2.7</b>	<b>TABLE: MAINS transformer</b>	<b>Form A.39</b>		N/A
4.4.2.7.2	Short circuit			N/A
14.6	MAINS transformers tested outside equipment			N/A
Type .....	:			—
Manufacturer .....	:			—
Test in equipment				
Test on bench				
Test repeated inside equipment (see 14.6)				
Optional – Insulation class (IEC 60085) of the lowest rated winding .....		:		—
Winding identification				
Type of Protector for winding (NOTE 1)				
Elapsed time				
Current, A primary				
secondary				
Winding temperature, °C primary				
(see NOTE 2) secondary				
Tissue paper / cheesecloth OK ? (Pass / Fail)				
Voltage tests (see NOTE 3)				
Primary to secondary	_____ V _____			
Primary to core	_____ V _____			
Secondary to secondary	_____ V _____			
Secondary to core	_____ V _____			
Verdict				
NOTE 1:	Primary fuse	- PF / ( )	A	
	Secondary fuse	- SF / ( )	A	
	Overtemperature protection	- OP / ( )	°C	
	Impedance protection	- Z		
NOTE 2:	Indicate method of measurement	- TC = with thermocouple		
		- R = resistance method		
	If resistance method is used, record resistance in cold and warm condition in Form A.26B.			
NOTE 3:	Record the voltage applied and the type of voltage (r.m.s. / d.c. / peak) and for results use NB = no breakdown or B = breakdown			
Supplementary information:				

IEC 61010-1				
Clause	Requirement — Test	Result — Remark		Verdict
<b>4.4.2.7</b>	<b>TABLE: MAINS transformer</b>	<b>Form A.40</b>		N/A
4.4.2.7.3	Overload tests (for MAINS transformers)			N/A
14.6	MAINS transformers tested outside equipment			N/A
Type .....				—
Manufacturer .....				—
Test in equipment				
Test on bench				
Test repeated inside equipment (see 14.6)				
Optional – Insulation class (IEC 60085) of the lowest rated winding .....				—
Winding identification				
Type of Protector for winding (NOTE 1)				
Elapsed time				
Current, A primary				
secondary				
Winding temperature, °C primary				
(see NOTE 2) secondary				
Tissue paper / cheesecloth OK ? (Pass / Fail)				
Voltage tests (see NOTE 3)				
Primary to secondary	_____ V _____			
Primary to core	_____ V _____			
Secondary to secondary	_____ V _____			
Secondary to core	_____ V _____			
Verdict				
NOTE 1:	Primary fuse	- PF / ( )	A	
	Secondary fuse	- SF / ( )	A	
	Overtemperature protection	- OP / ( )	°C	
	Impedance protection	- Z		
NOTE 2:	Indicate method of measurement	TC = with thermocouple		
		R = resistance method		
	If resistance method is used, record resistance in cold and warm condition in Form A.26B.			
NOTE 3:	Record the voltage applied and the type of voltage (r.m.s. / d.c. / peak) and for results use NB = no breakdown or B = breakdown			
Supplementary information:				



IEC 61010-1			
Clause	Requirement – Test	Result — Remark	Verdict

<b>Annex H</b>	<b>TABLE: Qualification of conformal coating for protection against pollution</b>	<b>Form A.42</b>	N/A
----------------	---	------------------	-----

Technical properties			
Manufacturer			—
Type			—
Meet requirements of ANSI / UL 746E	[yes / no]		
Manufacturer declaration of coating material	[yes / no]		
Operating temperature of coating	[ ] °C		
Comparative tracking index (CTI)	[ ]		
Insulation resistance	[ ] MΩ		
Dielectric strength	[ ] V		
UV resistance (if required)	[yes / no]		
Flammability rating			
Preparation of the test specimens conducted	[yes / no]		

Item	Test conditioning	Parameter	Td h	Samples						Verdict	Comments
				1	2	3	4	5	6		
1	Cold		24								
2	Dry heat		48								
3	Rapid temp. change										
4	Damp heat		24								
5	Adhesion of coating	5 N									
	Visual inspection										
6	Humidity		48								
7	Insulation resistance	≥ 100 MΩ									
	Visual inspection										

NOTE Td = Test duration time

Supplementary information:



IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

TABLE 1.A: List of components and circuits relied on for safety							P
Unique component reference or location	Application/function	Manufacturer / trademark (NOTE 1)	Type / model	Technical data (NOTE 2)	Standard	Mark(s) of conformity evidence of acceptance (NOTE 3 and 4)	
Power adapter	Power supply	Shenzhen HONOR Electronic Co., Ltd.	ADS-12EA-05 05010E	Input:100-240V, 50/60Hz, 0,3A Max. Output: 5 V d.c., 2 A	EN 61010-1 EN 60950-1	Test with appliance CB by UL DK-47521-A1-UL	
Plastic enclosure	Mechanical, fire enclosure	COVESTRO DEUTSCHLAND AG [PC RESINS]	FR3010 + (z)	Min. thickness: 1,5mm, 85°C, V-0 or better	UL 94	UL E41613	
RTC battery	RTC power	SEIKO INSTRUMENTS INC MICRO-ENERGY DIV	ML414H	3 V d.c., Max. charging current: 300mA, 1mAh	UL 1642	UL MH15628	
Lithium battery pack	Power supply	Dongguan Anyfine electronic Technology Co., Ltd	E097-27-1P1S18650	3,6 Vd.c., 3,35 Ah	IEC 62133-2	SGS test report no.: SHES190301213701	
Lithium battery cell	Power	LG CHEM, LTD	INR18650F1L or F1L / INR19/66	3,63 Vd.c., 3350 mAh	IEC 62133	CB by UL DK-45572-UL	
Laser diode	Laser source	Zhongshan Tianzhi optical technology Ltd.	TZ6X11D1-01	655 nm, 3,3 V d.c., 0,9 mA	IEC/EN 61010-1	Test with appliance	
LCD Panel	Display	JIANGXI HOLITECH TECHNOLOGY CO., LTD.	HIB024A080	2,4inch, TFT LCD, 3,2 Vd.c., 80 mA	IEC/EN 61010-1	Test with appliance	
NOTE → 1 List all different manufacturers of the above components → 4 asterisk indicates mark assuring agreed level of surveillance → 2 May include electrical, mechanical values → 3 List licence no or method of acceptance							



Details of: General View




Details of: General View





Details of: General View

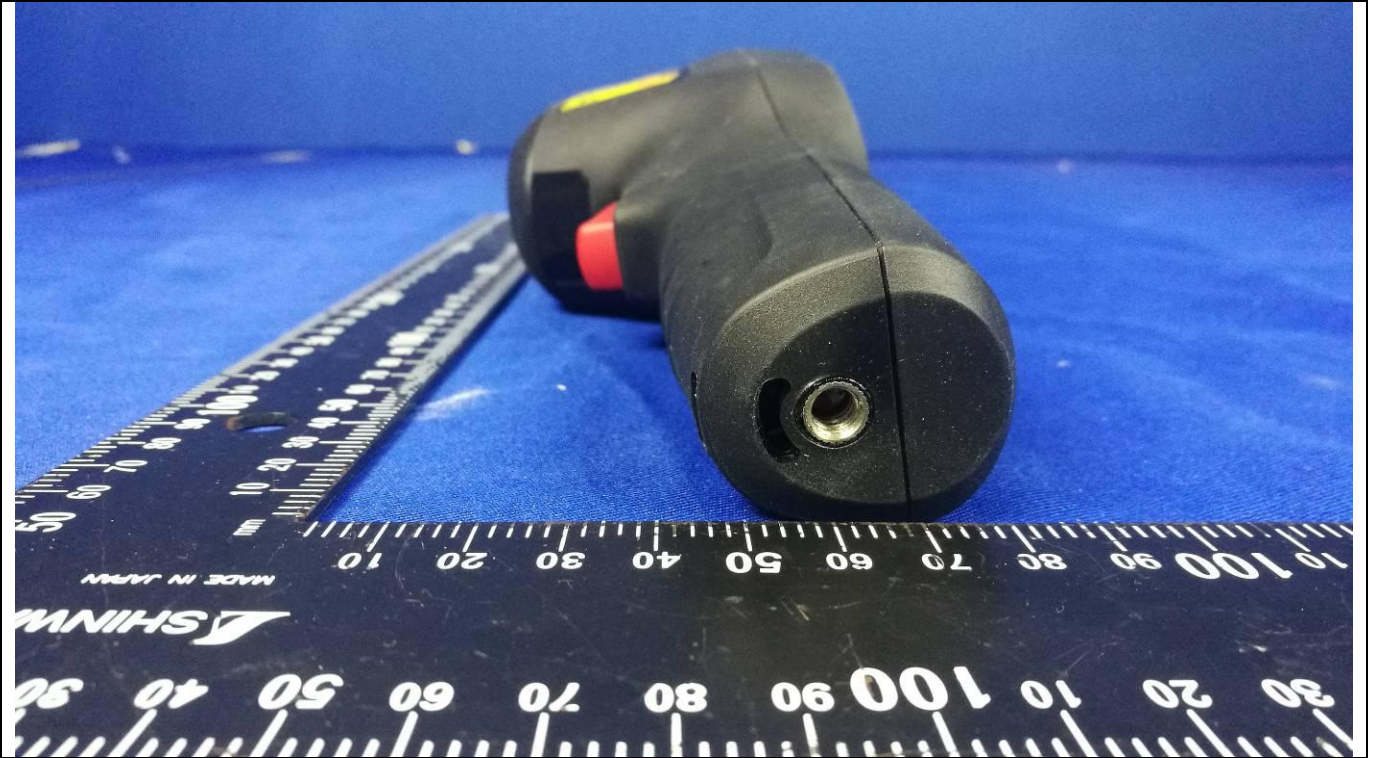

Details of: General View





Details of: General View




Details of: General View






Details of: Internal View

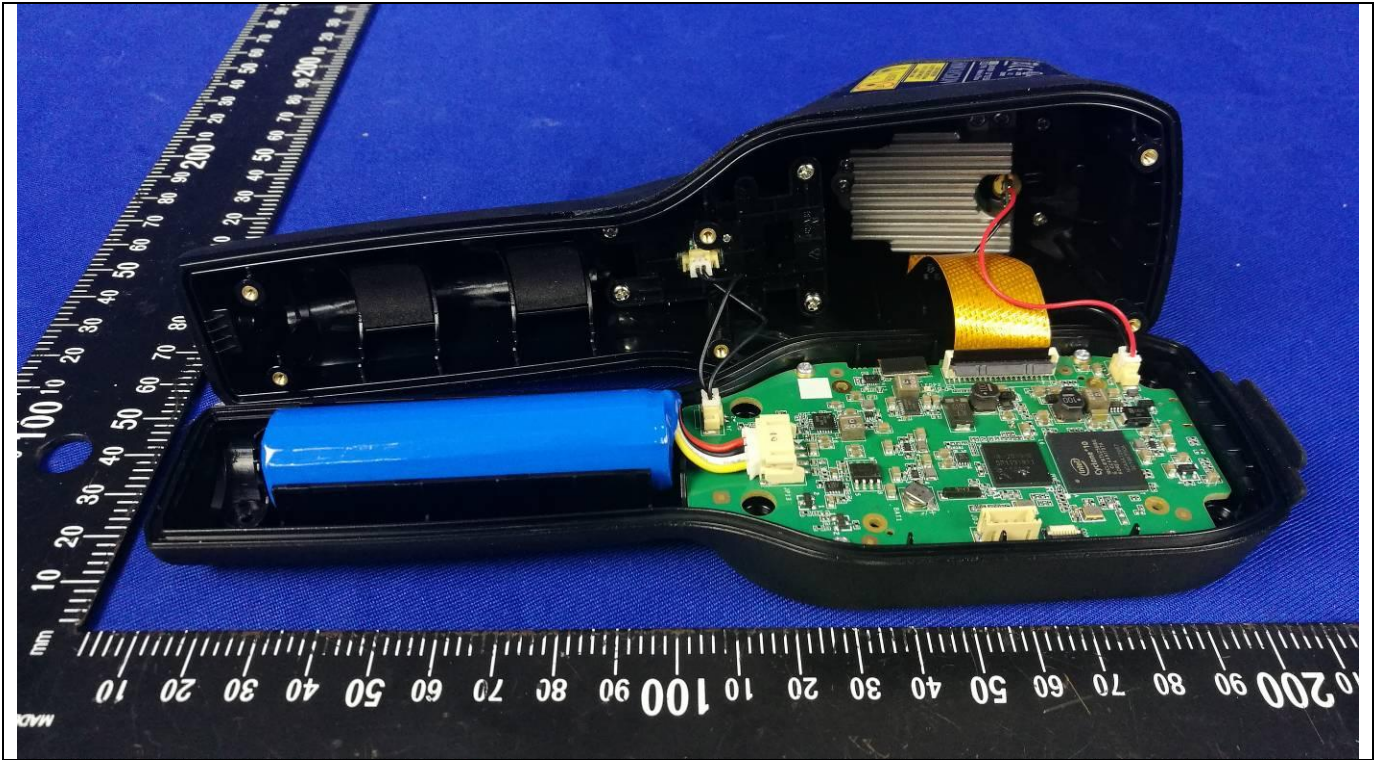


Details of: Top view of PCB

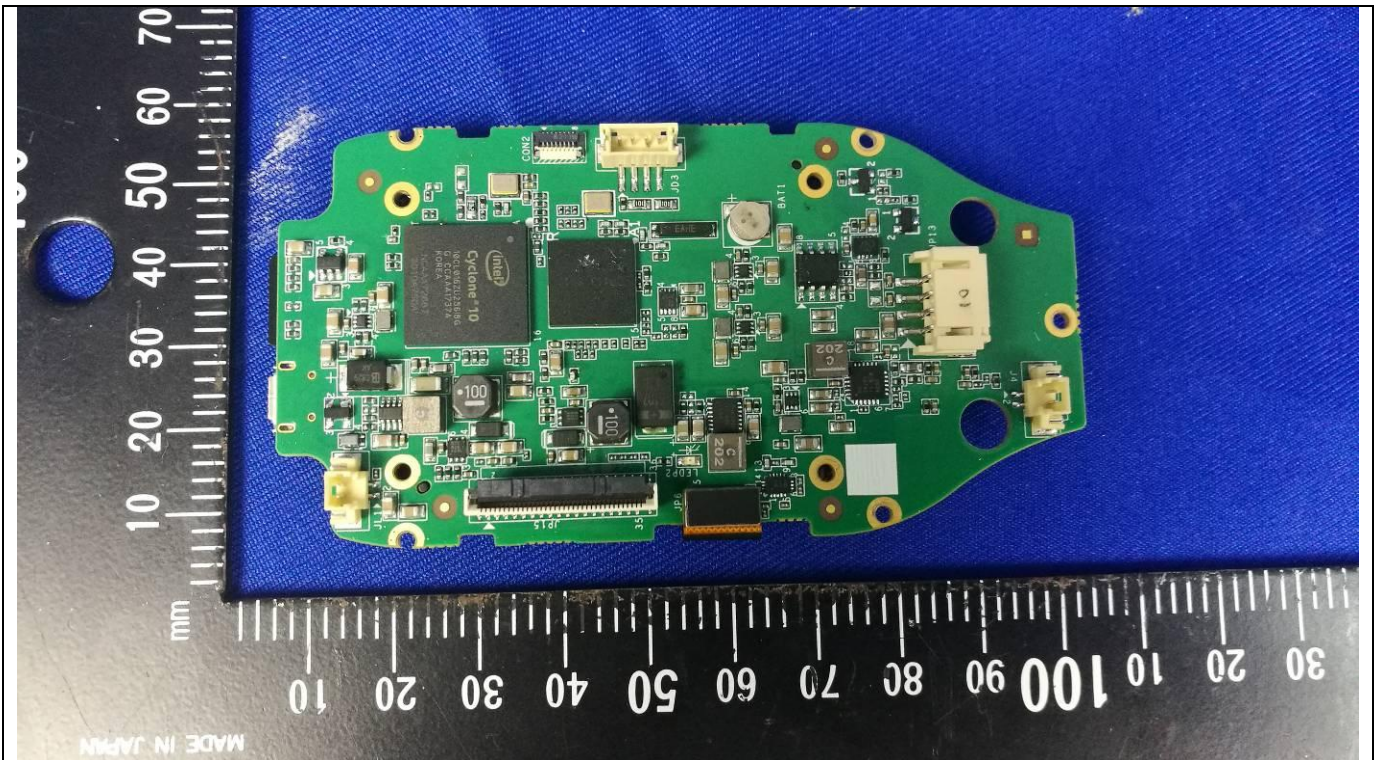




Details of: Internal View

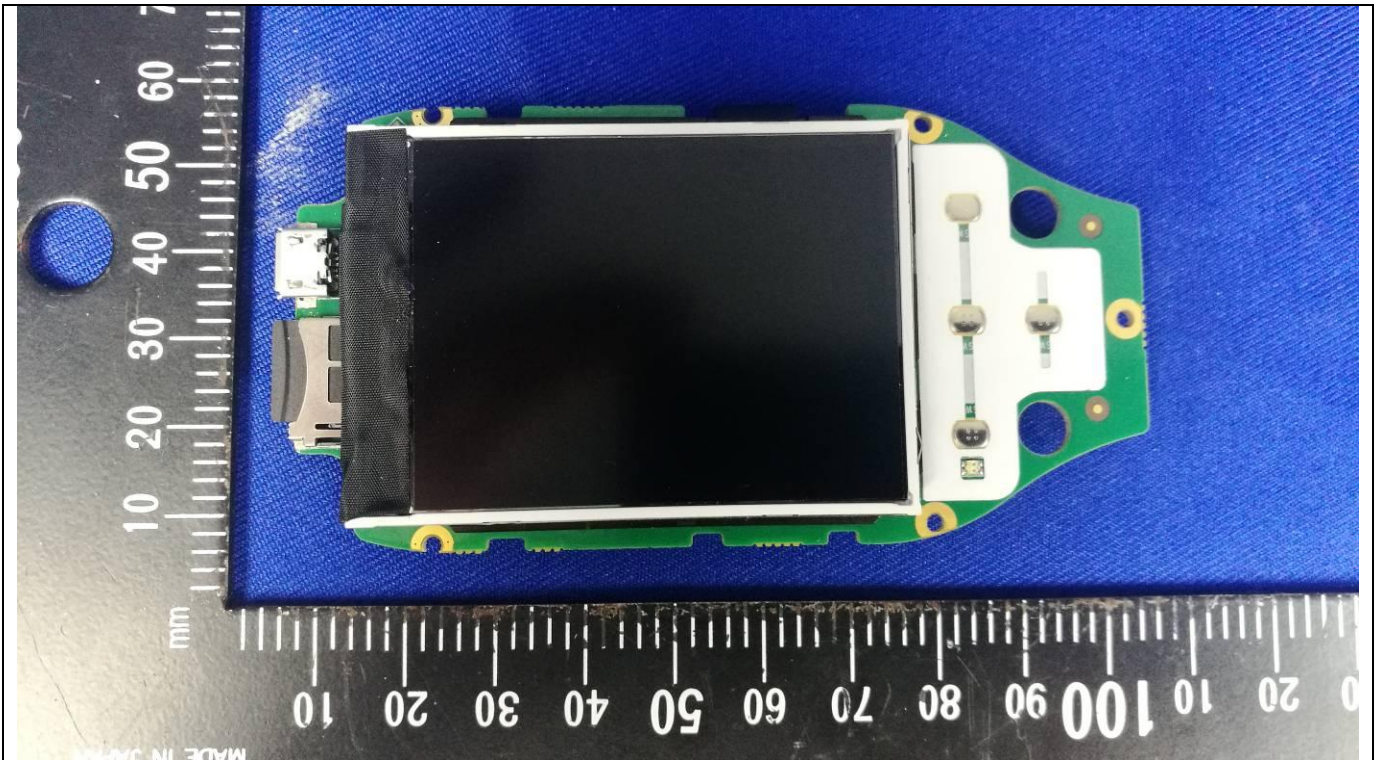


Details of: Internal View

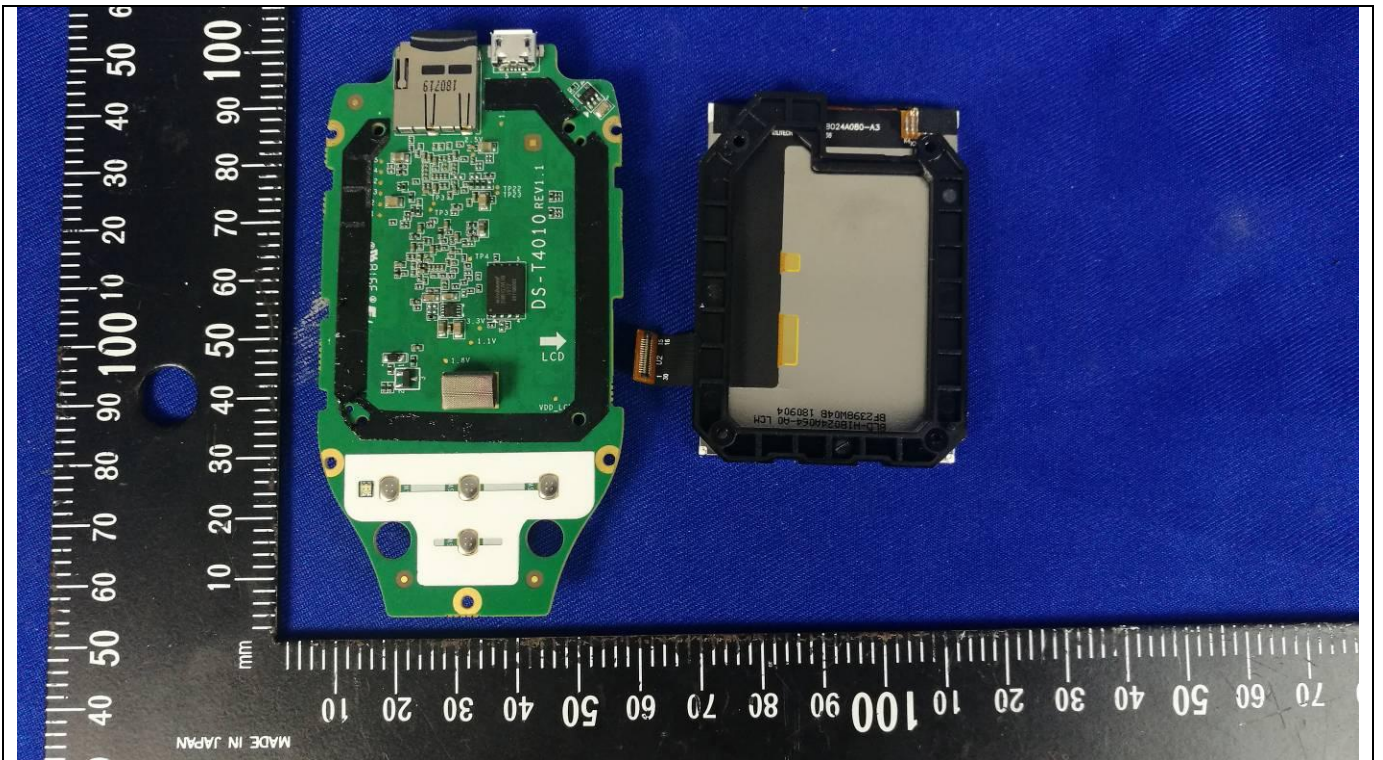




Details of: Internal View

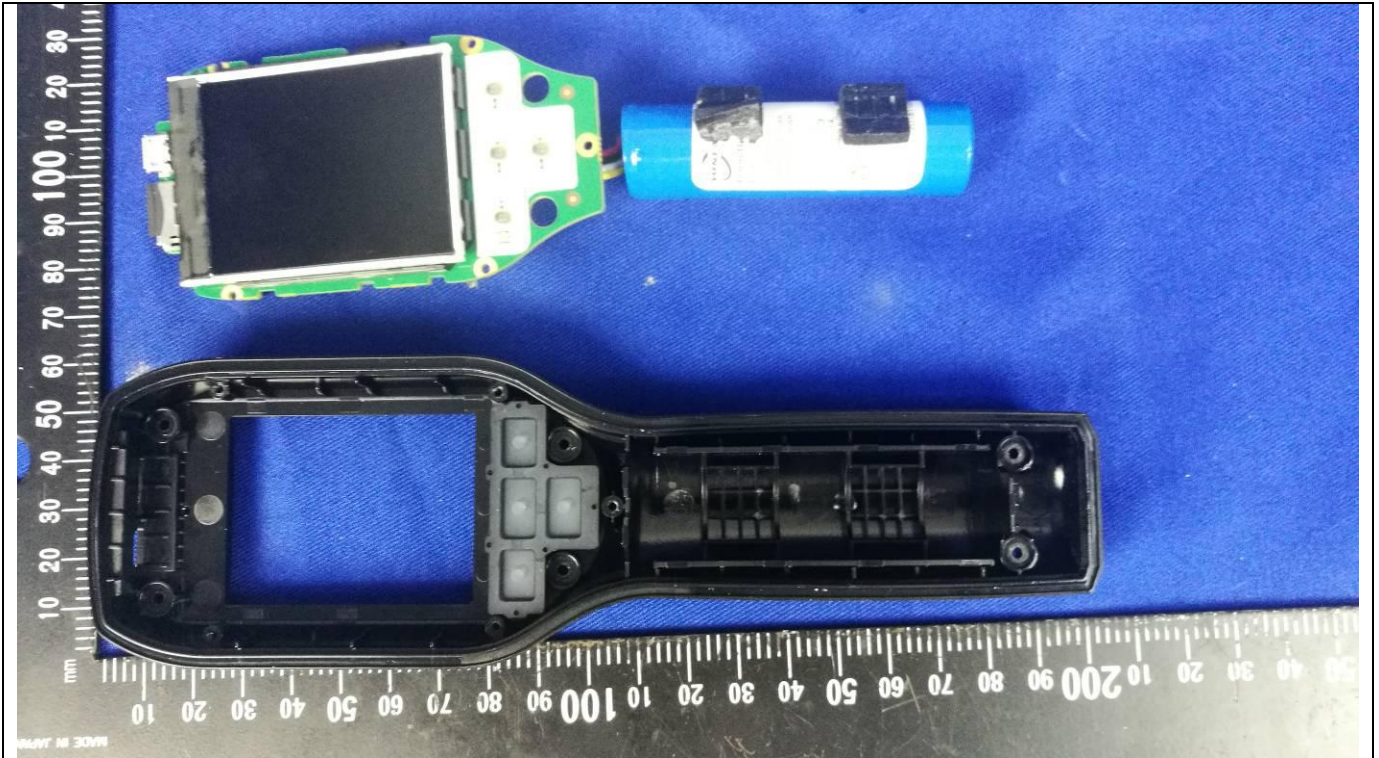


Details of: Internal View

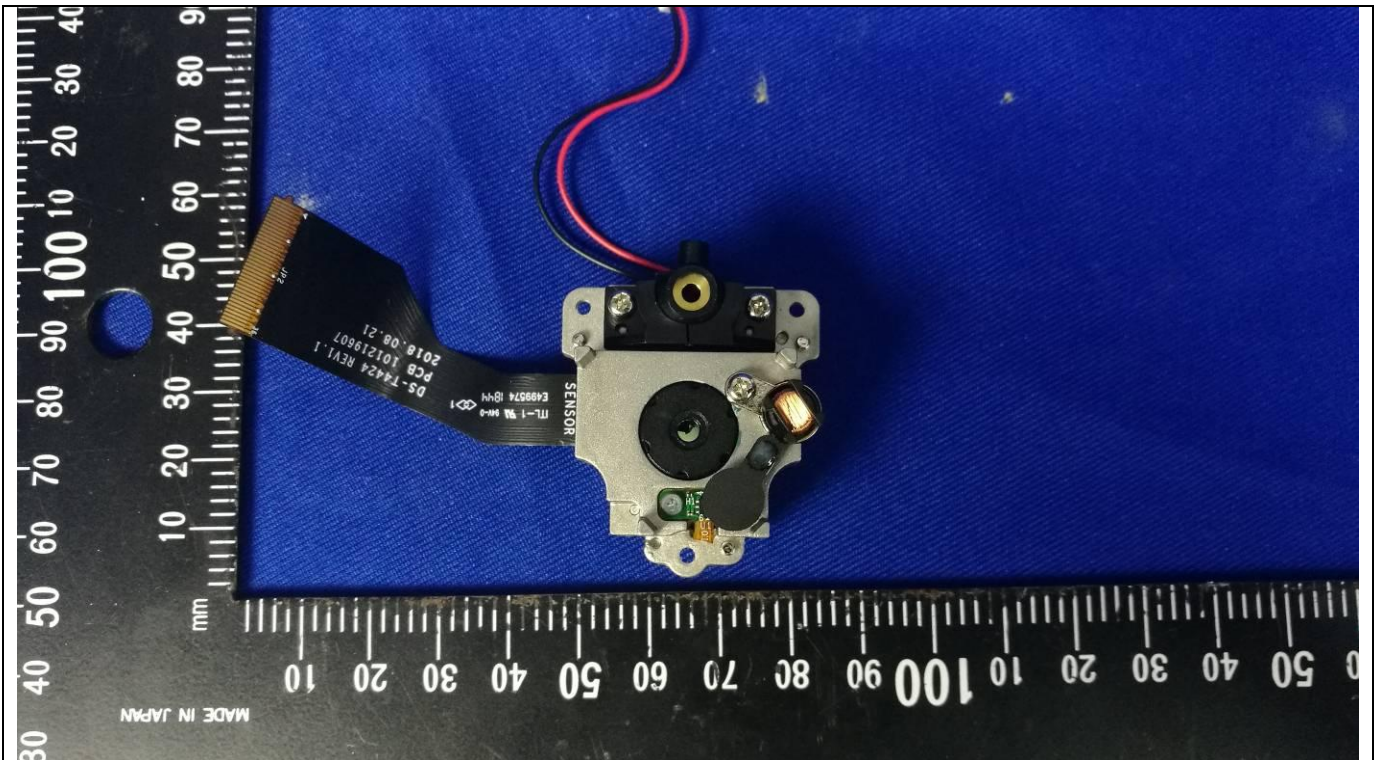





Details of: Internal View

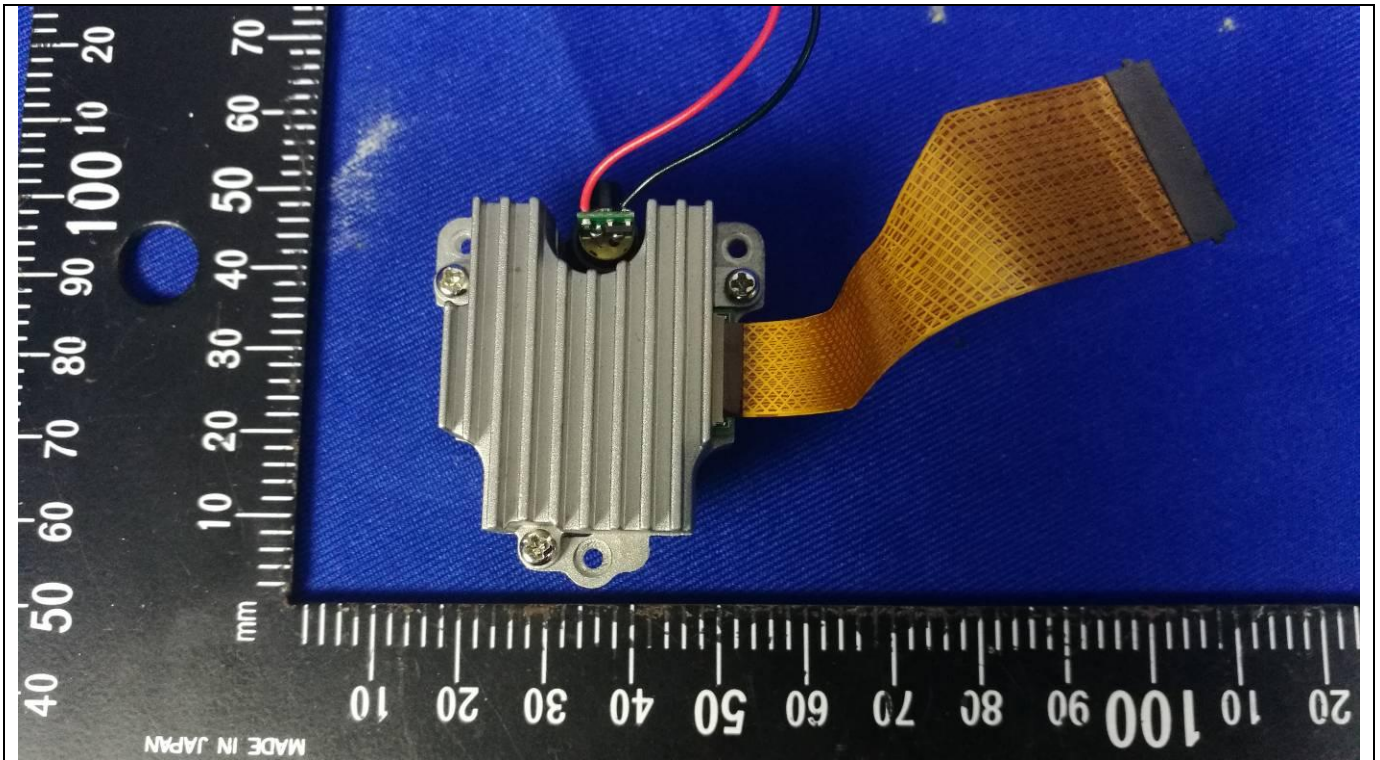

Details of: Internal View

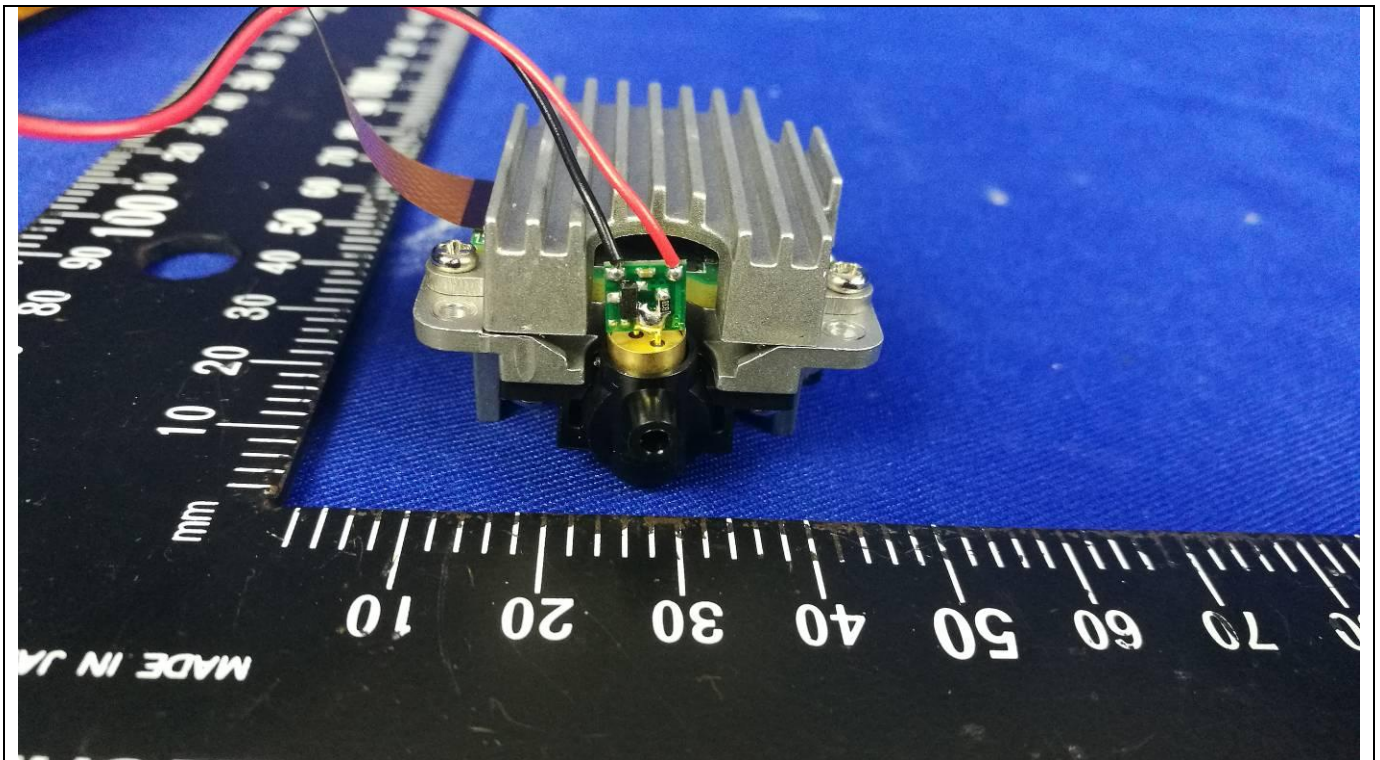

Details of: Internal View

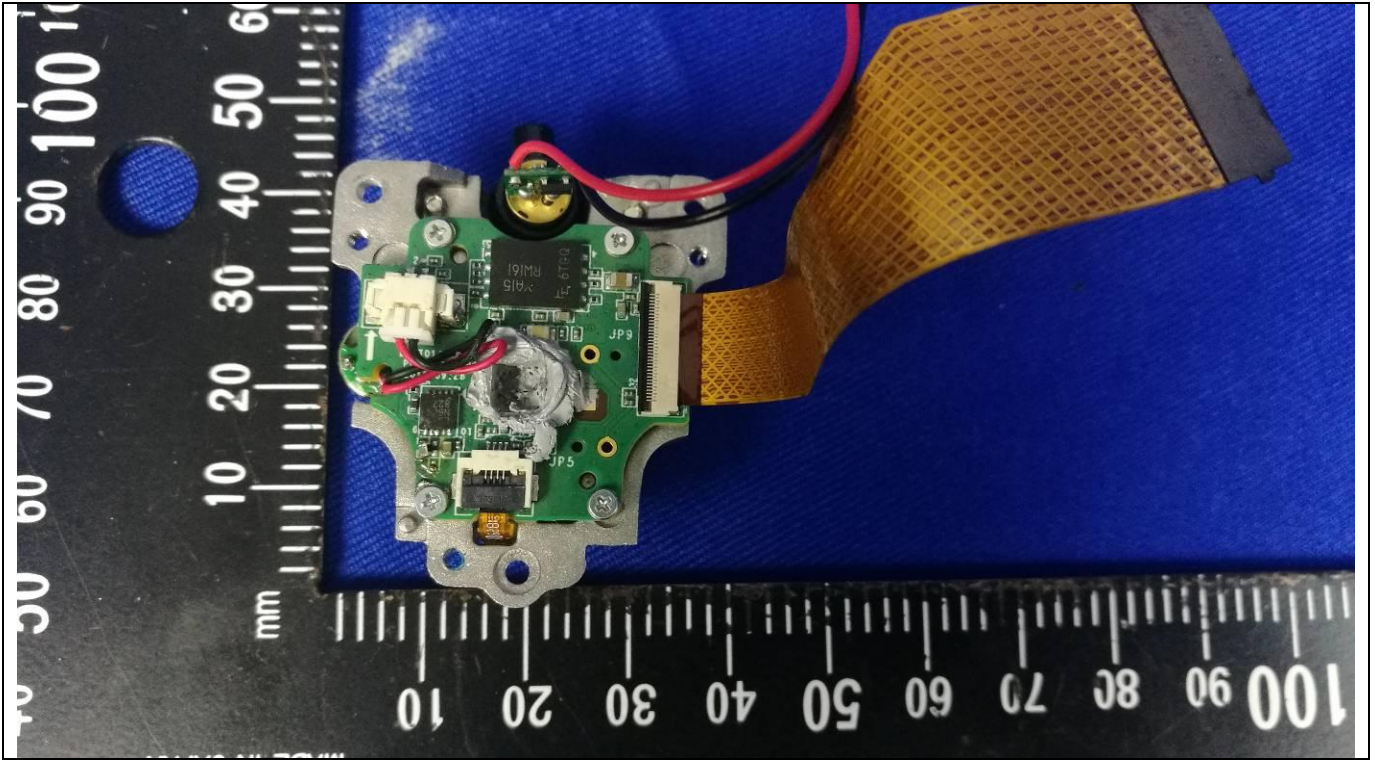

\*\*\*\*End of Attachment 1\*\*\*\*